

# **GeoPT47A — AN INTERNATIONAL PROFICIENCY TEST FOR ANALYTICAL GEOCHEMISTRY LABORATORIES — REPORT ON ROUND 47A (Silty Soil, NES-1) / December 2020**

**Peter C. Webb<sup>1\*</sup>, Philip J. Potts<sup>1</sup>, Michael Thompson<sup>2</sup> and Charles J. B. Gowing<sup>3</sup>**

<sup>1</sup>Formerly of the Faculty of Science, Technology, Engineering and Mathematics, The Open University, Walton Hall, Milton Keynes, MK7 6AA, UK.

<sup>2</sup>School of Biological and Chemical Sciences, Birkbeck University of London, Malet Street, London WC1E 7HX, UK.

<sup>3</sup>British Geological Survey, Keyworth, Nottingham, NG12 5GG, UK.

\*Corresponding author, Peter Webb: e-mail [geopt.iag@gmail.com](mailto:geopt.iag@gmail.com)

*Keywords:* proficiency testing, quality assurance, GeoPT, GeoPT47A, Round 47A, NES-1, Silty Soil, BGS

## **Abstract**

Results are presented for Round 47A of the International Association of Geoanalysts' Proficiency Testing programme for analytical geochemistry laboratories. The supplementary test material distributed in this round of GeoPT was the Silty Soil, NES-1, collected and processed under the direction of Dr Charles Gowing of the British Geological Survey. In this report, the data contributed by 92 laboratories are listed, together with an assessment of consensus values, consequent *z*-scores and charts to show the distribution of contributed results and the overall performance of participating laboratories.

## **Introduction**

This forty-seventh round of the international proficiency testing programme, GeoPT, was conducted in a similar manner to earlier rounds. However, exceptional circumstances associated with the coronavirus pandemic affected scheduling (see **Timetable** section below). The programme is designed to be part of the routine quality assurance procedures employed by analytical geochemistry laboratories. It is organised by the International Association of Geoanalysts and is conducted in accordance with a published protocol, recently revised (IAG, 2020). The overall aim of the programme is to provide participating laboratories with *z*-score information for their reported measurement results so that each laboratory can decide whether the quality of their data is satisfactory in relation both to their chosen fitness-for-purpose criteria and to the

results submitted by other laboratories contributing to the round. In circumstances where *z*-scores are unsatisfactory, a participating laboratory is encouraged to investigate for unsuspected analytical bias and to take corrective action if this appears justified.

## **Steering Committee for Round 47A:**

P.C. Webb (administrator and results assessor), P.J. Potts (results reviewer), M. Thompson (statistical advisor), C.J.B. Gowing (distribution manager and supplier of NES-1).

## **Timetable for Round 47A:**

The coronavirus pandemic caused postponement of the mailing of test materials for Round 47A (originally scheduled for spring 2020), so that the interval after the previous round was extended from 6 to 11 months. The scheduled reporting window was extended by 10 days to allow for delayed deliveries.

Distribution of sample: August 2020

Results submission deadline: 30th November 2020

Release of report: January 2021

## **Test material details**

**GeoPT47A:** The Silty Soil test material, NES-1, was collected from the soil horizon overlying Old Red Sandstone deposits from Moorpark, Co. Cork, in the Republic of Ireland and processed at the British Geological Survey, Keyworth, under the direction of Dr Charles Gowing. The test material was evaluated for

homogeneity by the originator, and an evaluation of the results showed that this material was suitable for use in this proficiency test.

### Submission of results

For GeoPT47A (NES-1), a total of 3146 results are listed in Table 1 as submitted by 92 laboratories. Measurement results that were designated by the participating laboratory as data quality 1 (see **Z-score analysis section** below for explanation) are shown in **bold** and those specified as data quality 2 are shown underlined. Results from all laboratories submitting data were used to assess respective consensus values. It is gratifying that no value of '0' (i.e., zero) was reported for this round. However, it is suspected that several laboratories reported results for C(org), C(tot), F, S and even Zr in units of g/100g instead of mg/kg. We must remind analysts reporting results that measurements of all trace constituents should be reported in mg/kg. Analysts should be aware that suspected invalid results **cannot be altered or removed** once they have been submitted and that their corresponding z-scores will be adversely affected.

### Assigned values and results summary

Following procedures described in earlier rounds and detailed fully in the GeoPT protocol (IAG, 2020), robust statistical procedures were used to derive consensus values for measurands in this test material: these consensus values being judged to be the best available estimates of the true composition of the test material. Values were assigned on the basis that: i) sufficient laboratories (15 or more) had contributed data for estimating the consensus, ii) visual assessment gave confidence that a substantial proportion of the results distribution was symmetrically disposed about the consensus value, iii) the ratio of the uncertainty in the location estimate to the target precision was an acceptably small value, and iv) an evaluation of measurement results by procedure – including both methods of analysis and sample preparation – indicated that no significant procedural bias was discernible amongst measurement results from which the consensus was derived. Where these criteria were largely, but not

fully met, values were credited with 'provisional' rather than 'assigned' status.

These assessments involve examining the distribution of results from barcharts of data contributed for each measurand (as presented in Figures 1 and 2). In addition, when appropriate, a variety of plots permitting discrimination of data by method of analysis and by sample preparation procedure, as developed by Thomas Meisel using the Shiny App (<https://www.shinyapps.io>) and linked to the statistical package 'R', were also examined. This enabled us, when necessary, to refine the selection of consensus values by taking account of data distributions according to analytical procedure.

Consensus values derived from contributed data were provided by the Huber robust mean in only 4 instances. Although outliers can be accommodated by this procedure, frequently, as when a dataset is skewed, it does not provide a satisfactory estimation of the consensus. In such circumstances, the median is often a more appropriate robust estimator and was employed in 19 cases. For more severely skewed and strongly tailed datasets, even the median may not be satisfactory and a mode can often be a much more effective means of estimating the location of the consensus. In this round the use of modes as consensus location estimators was preferred in 31 cases, and in 23 of these, distributions were compatible with the conditions outlined above to justify their designation as assigned values. The procedure used to determine modes was most often that described by Thompson (2017) involving the estimation of the mass fraction that corresponds to the maximum value of the kernel density distribution for the dataset. Such modes derived by bootstrapping provide robust estimates of consensus locations representing the most coherent part of data distributions where data are symmetrically disposed, although the dataset as a whole may be asymmetric.

Table 2 lists assigned and provisional values for 10 major components and 44 trace elements in GeoPT47A (NES-1). Barcharts that were judged to have satisfactory distributions for consensus values to be designated as assigned or provisional values, enabling z-scores to be calculated, are shown in Figure 1. These 54 measurands

of GeoPT47A listed in Table 2 are for the analytes: SiO<sub>2</sub>, TiO<sub>2</sub>, Al<sub>2</sub>O<sub>3</sub>, Fe<sub>2</sub>O<sub>3</sub>T, MnO, MgO, CaO\*, K<sub>2</sub>O, P<sub>2</sub>O<sub>5</sub>, LOI\*, As\*, Ba, Be, Bi\*, Cd\*, Ce, Co, Cr\*, Cs, Cu, Dy, Er, Eu, Ga\*, Gd, Hf\*, Ho, La, Li, Lu, Mo, Nb, Nd, Ni, Pb, Pr, Rb, Sb\*, Sc, Sm, Sn\*, Sr, Ta, Tb, Th, Tl, Tm, U, V\*, W\*, Y, Yb, Zn and Zr. Of these, the measurands of the 12 analytes marked '\*' were credited only with provisional status. Such instances of provisional status were identified because either: i) a relatively small number of results (less than 15, but usually more than 9) contributed to the consensus, or ii) the results were unduly dispersed in relation to the target value, or iii) the distribution of results was significantly skewed.

Bar charts for the 15 analytes: Fe(II)O, Na<sub>2</sub>O, H<sub>2</sub>O<sup>+</sup>, Ag, Br, C(org), C(tot), Cl, F, Ge, Hg, In, S, Se and Te are plotted in Figure 2 for information only, as the data were either insufficient in number, or the distribution was too highly skewed or too variable for the reliable determination of a consensus for the estimation of z-scores.

## Data review

Although some datasets in this round were largely symmetrically disposed, with relatively little dispersion of the data, many datasets were skewed, featuring variable degrees of asymmetry, and requiring estimation of the consensus using median values and modes.

For a number of constituents strongly low-tailed distributions were apparent, especially for Hf and Zr, but also to varying extents for Dy, Er, Ho, Lu, Nb, Tb, Tm, Y and Yb. Most of these low values were reported by laboratories using acid digestion prior to ICP-MS or ICP-AES measurement. Such observations are comparable to those reported for GeoPT31 (SdAR-1) by Potts et al (2015), where digestion recoveries were incomplete for a similar range of analytes. In this case, as for SdAR-1, the suspicion is that accessory zircon is responsible, since it frequently hosts not only Zr, but Hf and HREEs and is particularly susceptible to incomplete dissolution.

High tails were noted for Al<sub>2</sub>O<sub>3</sub>, MnO, CaO, Ag, Ba, Be, Bi, Ce, Co, Cs, Cu, Ga, La, Mo, Ni, Pb, Sb, Sc, Sn, Sr, Th, U, V and W. Some of these, such as those of CaO,

Ce, Ga, La and Pb are the result of relatively poor precision of values reported by particular measurement procedures, frequently those derived by XRF (but not obviously so in the case of CaO). There is a consequent tendency for such values to display a positive bias, especially when reported at mass fractions close to, and in some cases below, a realistic detection limit for the measurement procedure, such as for As, Mo, U, Sc, Sn, Th and W. For Al<sub>2</sub>O<sub>3</sub>, MnO and to a lesser extent for CaO the high values were largely from XRF powder pellet measurements, as were several of the values in the contrasting low tail exhibited by SiO<sub>2</sub>. In one case, for Mo, high values appear to reflect a preponderance of preparation by fusion prior to ICP-MS measurement, whereas acid digestions have a more coherent distribution. Unusually, a high tail is noted for Sr, largely due to XRF values, although they are also distributed throughout and should not be affected by proximity to the detection limit for Sr.

In some sets of results, notably those of MnO, MgO, CaO and P<sub>2</sub>O<sub>5</sub>, stepped distributions are apparent owing to over-rounding of much of the data. Our firm recommendation is that minor components should be quoted to at least three decimal places in order for the statistical procedures to more effectively define the consensus. Similar logic also applies when any components (such as CaO) are reported at low mass fractions.

For several trace elements, it is noteworthy that the reported data exhibit a high degree of coherence and consistency although there are insufficient data to satisfy our criteria for establishment of values that would permit z-scores to be quoted. In such cases information values may be recognised, including 14.9 mg/kg for Br, 0.082 mg/kg for Hg and 0.027 mg/kg for In.

## Z-score analysis

As in previous rounds, laboratories were invited to choose one of two performance standards against which their analytical results would be judged:

**Data quality 1** for laboratories working to a 'pure geochemistry' standard of performance, where analytical results are designed for geochemical research and where

care is taken to provide data of high precision and accuracy, sometimes at the expense of a reduced sample throughput rate. For GeoPT47A, 1418 results of data quality 1 were submitted.

**Data quality 2** for laboratories working to an 'applied geochemistry' standard of performance, where, although precision and accuracy are still important, the main objective is to provide results on large numbers of samples collected, for example, as part of geochemical mapping projects or geochemical exploration programmes. For GeoPT47A, 1728 results of data quality 2 were submitted.

The target standard deviation ( $H_a$ ) for each measurand assessed was calculated from a modified form of the Horwitz function as follows:

$$H_a = k \cdot X_a^{0.8495}$$

Where  $X_a$  is the mass fraction of the element; the factor  $k = 0.01$  for pure geochemistry laboratories and  $k = 0.02$  for applied geochemistry laboratories.

Z-scores were calculated for each elemental measurement submitted by each laboratory from:

$$z = [X - X_a] / H_a$$

Where  $X$  is the contributed measurement result,  $X_a$  is the assigned value and  $H_a$  is the target standard deviation (all as mass fractions). Z-scores for results contributed to GeoPT47A are listed in Table 3. Results designated as data quality 1 are shown in bold: results of data quality 2 are shown underlined. Z-scores derived from provisional values of measurands are shown in italics.

Participating laboratories are invited to assess their performance using the following criteria:-

Z-score results in the range  $-2 < z < 2$  are considered to be 'satisfactory' (in the sense that no action is called for by the participant). If the z-score for an element falls outside this range, especially if it is outside the range  $-3 < z < 3$ , laboratories are advised to examine their procedures, and if necessary, take action to ensure that determinations are not subject to unsuspected analytical bias.

## Overall performance

A summary of the overall performance of individual laboratories for this round is plotted in multiple z-score charts in Figure 3. In these charts, the z-score performance for each element is distinguished by symbols that make it easy to identify whether the results were satisfactory or gave z-scores that exceeded the action limits. This chart is designed to help individual laboratories judge their overall performance in this proficiency testing round. Participants should always review their z-scores in accordance with their own fitness-for-purpose criteria.

## Participation in future rounds

The benefit from proficiency testing arises from regular participation and laboratories are invited to contribute to Round 48, the test sample for which was distributed during September 2020. This round was delayed from autumn 2020 and will take place in early spring 2021.

## Acknowledgements

The authors once again thank Andrea Mills (BGS) for much-valued assistance in distributing these samples and Thomas Meisel for development of procedures involving the Shiny App which has greatly assisted the investigation of data according to analytical procedure and facilitated analysis of datasets involving modes derived according to Thompson (2017).

## References

- IAG (2020)** Protocol for the operation of the GeoPT Proficiency testing scheme. International Association of Geoanalysts (Keyworth, UK), 18pp.  
<http://www.geoanalyst.org/wp-content/uploads/2020/07/GeoPT-revised-protocol-2020.pdf>.
- Potts P.J., Webb P.C. and Thompson M. (2015)** Bias in the determination of Zr, Y and rare earth element concentrations in selected silicate rocks by ICP-MS when using some routine acid dissolution procedures: Evidence from the GeoPT proficiency testing programme. *Geostandards and Geoanalytical Research*, 39, 403–416.
- Thompson, M. (2017)** On the role of the mode as a location parameter for the results of proficiency tests in chemical measurement. *Anal. Methods*, 9, p.5534-5540.

## **ADDENDUM**

### **— IMPORTANT NOTICES TO ANALYSTS**

#### **Change in uncertainty estimation:**

A change has been made to the algorithm for the estimation of uncertainty for median values. The revised procedure has been implemented for the first time in this round (GeoPT47/47A). As described in the revised GeoPT protocol (IAG, 2020), median uncertainties are increased by a factor of 1.2533. Therefore, when comparing uncertainties from this and future rounds with those from past rounds those uncertainty values previously reported for medians should be increased by this factor.

#### **Explicit advice to analysts regarding reporting of procedures involving ignition and fusion:**

Note that too many laboratories are still listing their procedure for determining LOI as the same as that employed for major elements, rather than providing separate, specific details. We must remind analysts that it is important to provide information that is appropriate for every analyte. Indeed, analysts reporting measurement results for procedures involving fusion, sintering or ignition, and in particular, LOI determinations, should specify the correct method used and give details both of the temperature used and where appropriate, the end-point criterion, e.g., the duration of ignition. This information should be supplied in the description of the relevant **Procedure**, as **Additional Details**.

We recommend that details of gravimetric procedures are included under **Analytical Technique details** rather than under **Sample Preparation details**. For gravimetric analysis, other than drying, which should in any case be carried out according to our instructions, there is no other sample preparation involved.

#### **References of more general relevance**

**Potts, P.J., Thompson, M., and Webb, P.C. (2015)** The Reliability of Assigned Values from the GeoPT Proficiency Testing Programme from an Evaluation of Data for Six Test Materials that have been Characterised as Certified Reference Materials. *Geostandards and Geoanalytical Research*, **39**, 407–417.

**Potts, P.J., Webb, P.C. and Thompson M. (2019)** The GeoPT proficiency testing programme as a scheme for the certification of geological reference materials. *Geostandards and Geoanalytical Research*, **43**, 409–418.

**Webb, P.C., Potts P.J., Thompson M., Wilson, S.A. and Gowing, C.J.B. (2019)** The long-term robustness and stability of consensus values as composition location estimators for a typical geochemical test material in the GeoPT proficiency testing programme. *Geostandards and Geoanalytical Research*, **43**, 397–408.

**Potts, P.J. and Webb, P.C (2019)** An Evaluation of Methods for Assessing the Competence of Laboratories Based on Performance in the GeoPT Proficiency Testing Scheme. *Geostandards and Geoanalytical Research*, **43**, 217–229.

## **Appendix 1**

Publication status of proficiency testing reports.  
Previous reports are available for download from the IAG website (<http://www.geoanalyst.org/>).

### **GeoPT1**

Thompson M., Potts P.J., Kane J.S. and Webb P.C. (1996) GeoPT1. International proficiency test for analytical geochemistry laboratories - Report on round 1. *Geostandards Newsletter: The Journal of Geostandards and Geoanalysis*, **20**, 295–325.

### **GeoPT2**

Thompson M., Potts P.J., Kane J.S., Webb P.C. and Watson, J.S. (1998) GeoPT2. International proficiency test for analytical geochemistry laboratories - Report on round 2. *Geostandards Newsletter: The Journal of Geostandards and Geoanalysis*, **22** 127–156.

### **GeoPT3**

Thompson M., Potts P.J., Kane J.S. and Chappell B.W. (1999a) GeoPT3. International proficiency test for analytical geochemistry laboratories - Report on round 3. *Geostandards Newsletter: The Journal of Geostandards and Geoanalysis*, **23**, 87–121.

### **GeoPT4**

Thompson M., Potts P.J., Kane J.S., Webb P.C. and Watson J.S. (1999b) GeoPT4. International proficiency test for analytical geochemistry laboratories - Report on round 4. Published in the electronic version of *Geostandards Newsletter: The Journal of Geostandards and Geoanalysis* (Summer 2000).

### **GeoPT5**

Thompson M., Potts P.J., Kane J.S., and Wilson S. (1999c) GeoPT5. International proficiency test for analytical geochemistry laboratories - Report on round 5. Published in the electronic version of *Geostandards Newsletter: The Journal of Geostandards and Geoanalysis* (Summer 2000).

## Appendix 1 (Cont'd)

### GeoPT6

Potts P.J., Thompson M., Kane J.S., Webb P.C. and Carignan J. (2000) GEOPT6 - an international proficiency test for analytical geochemistry laboratories - report on round 6 (OU-3: Nanhron microgranite) and 6A (CAL-S: CRPG limestone). International Association of Geoanalysts: Unpublished report.

### GeoPT7

Potts P.J., Thompson M., Kane J.S., and Petrov L.L. (2000) GEOPT7 - an international proficiency test for analytical geochemistry laboratories - report on round 7 (GBPG-1 Garnet-biotite plagiogneiss). International Association of Geoanalysts: Unpublished report.

### GeoPT8

Potts P.J., Thompson M., Kane J.S., Webb, P.C. and Watson J.S. (2000) GEOPT8 - an international proficiency test for analytical geochemistry laboratories - report on round 8 / February 2001 (OU-4 Penmaenmawr microdiorite). International Association of Geoanalysts: Unpublished report.

### GeoPT9

Potts P.J., Thompson M., Webb, P.C. and Watson J.S. (2001) GEOPT9 - an international proficiency test for analytical geochemistry laboratories - report on round 9 / July 2001 (OU-6 Penrhyn slate). International Association of Geoanalysts: Unpublished report.

### GeoPT10

Potts P.J., Thompson M., Webb, P.C., Watson J.S. and Wang Yimin (2001) GEOPT10 - an international proficiency test for analytical geochemistry laboratories - report on round 10 / December 2001 (CH-1 Marine sediment). International Association of Geoanalysts: Unpublished report.

### GeoPT11

Potts P.J., Thompson M., Chenery S.R., Webb, P.C. and Watson J.S. (2002) GEOPT11 - an international proficiency test for analytical geochemistry laboratories - report on round 11 / July 2002 (OU-5 Leatton dolerite). International Association of Geoanalysts: Unpublished report.

### GeoPT12

Potts P.J., Thompson M., Chenery S.R., Webb, P.C. and Batjargal B. (2003) GEOPT12 - an international proficiency test for analytical geochemistry laboratories - report on round 12 / January 2003 (GAS Serpentinite). International Association of Geoanalysts: Unpublished report.

### GeoPT13

Potts P.J., Thompson M., Chenery S.R., Webb, P.C. and Kaspar H.U. (2003) GEOPT13 - an international proficiency test for analytical geochemistry laboratories - report on round 13 / July 2003 (Köln Loess). International Association of Geoanalysts: Unpublished report.

### GeoPT14

Potts P.J., Thompson M., Chenery S.R., Webb, P.C. and B. Batjargal (2004) GEOPT14 - an international proficiency test for analytical geochemistry laboratories - report on round 14 / January 2004 (OShBO - alkaline granite). International Association of Geoanalysts: Unpublished report.

### GeoPT15

Potts P.J., Thompson M., Chenery S.R., Webb, P.C. and Wang Yimin (2004) GEOPT15 - an international proficiency test for analytical geochemistry laboratories - report on round 15 / June 2004 (Ocean floor sediment MSAN). International Association of Geoanalysts: Unpublished report.

### GeoPT16

Potts P.J., Thompson M., Webb, P.C. and S.Wilson (2005) GeoPT16 - an international proficiency test for analytical geochemistry laboratories - report on round 16 / February 2005 (Nevada basalt, BNV-1). International Association of Geoanalysts: Unpublished report.

### GeoPT17

Potts P.J., Thompson M., Webb, P.C. and J. Nicholas Walsh (2005) GeoPT17 - an international proficiency test for analytical geochemistry laboratories - report on round 17 / July 2005 (Calcareous sandstone, OU-8). International Association of Geoanalysts: Unpublished report.

### GeoPT18

Webb, P.C., Thompson M., Potts P.J. and L. Paul Bedard (2006) GeoPT18 - an international proficiency test for analytical geochemistry laboratories - report on round 18 / Jan 2006 (Quartz Diorite, KPT-1). International Association of Geoanalysts: Unpublished report.

### GeoPT19

Webb, P.C., Thompson M., Potts P.J. and B. Batjargal (2006) GeoPT19 - an international proficiency test for analytical geochemistry laboratories - report on round 19 / July 2006 (Gabbro, MGR-N). International Association of Geoanalysts: Unpublished report.

### GeoPT20

Webb, P.C., Thompson M., Potts P.J. and M. Burnham (2007) GeoPT20 - an international proficiency test for analytical geochemistry laboratories - report on round 20 / Jan 2007 (Ultramafic rock, OPY-1). International Association of Geoanalysts: Unpublished report.

### GeoPT21

Webb, P.C., Thompson M., Potts P.J. and B. Batjargal (2007) GeoPT21 - an international proficiency test for analytical geochemistry laboratories - report on round 21 / July 2007 (Granite, MGT-1). International Association of Geoanalysts: Unpublished report.

### GeoPT22

Webb, P.C., Thompson, M., Potts, P.J. and Batjargal, B. (2008) GeoPT22 - an international proficiency test for analytical geochemistry laboratories - report on round 22 / January 2008 (Basalt, MBL-1). International Association of Geoanalysts: Unpublished report.

### GeoPT23

Webb, P.C., Thompson, M., Potts, P.J., Watson, J.S. and Kriete, C. (2008) GeoPT23 - an international proficiency test for analytical geochemistry laboratories - report on round 23 / September 2008 (Separation Lake pegmatite, OU-9) and 23A (Manganese nodule, FeMn-1). International Association of Geoanalysts: Unpublished report.

### GeoPT24

Webb, P.C., Thompson, M., Potts, P.J. and Watson, J.S. (2009) GeoPT24 - an international proficiency test for analytical geochemistry laboratories - report on round 24 / January 2009 (Longmyndian greywacke, OU-10). International Association of Geoanalysts: Unpublished report.

### GeoPT25

Webb, P.C., Thompson, M., Potts, P.J. and Enzweiler, J. (2009) GeoPT25 - an international proficiency test for analytical geochemistry laboratories - report on round 25 / July 2009 (Basalt, HTP-1). International Association of Geoanalysts: Unpublished report.

### GeoPT26

Webb, P.C., Thompson, M., Potts, P.J. and Loubser, M. (2010) GeoPT26 - an international proficiency test for analytical geochemistry laboratories - report on round 26 / January 2010 (Ordinary Portland cement, OPC-1). International Association of Geoanalysts: Unpublished report.

### GeoPT27

Webb, P.C., Thompson, M., Potts, P.J. and Batjargal, B. (2010) GeoPT27 - an international proficiency test for analytical geochemistry laboratories - report on round 27 / July 2010 (Andesite, MGL-AND). International Association of Geoanalysts: Unpublished report.

## Appendix 1 (Cont'd)

### GeoPT28

Webb, P.C., Thompson, M., Potts, P.J. and Wilson, S. (2011)  
GeoPT28 - an international proficiency test for analytical geochemistry laboratories - report on round 28 / January 2011 (Shale, SBC-1). International Association of Geoanalysts: Unpublished report.

### GeoPT29

Webb, P.C., Thompson, M., Potts, P.J. and Wilson, S. (2011)  
GeoPT29 - an international proficiency test for analytical geochemistry laboratories - report on round 29 / July 2011 (Nepheline, NKT-1). International Association of Geoanalysts: Unpublished report.

### GeoPT30

Webb, P.C., Thompson, M., Potts, P.J., Long, D. and Batjargal, B. (2012)  
GeoPT30 - an international proficiency test for analytical geochemistry laboratories - report on round 30 / January 2012 (Syenite, CG-2) and 30A (Limestone, ML-2). International Association of Geoanalysts: Unpublished report.

### GeoPT31

Webb, P.C., Thompson, M., Potts, P.J and Wilson, S. (2012)  
GeoPT31 - an international proficiency test for analytical geochemistry laboratories - report on round 31 / July 2012 (Modified river sediment, SdAR-1). International Association of Geoanalysts: Unpublished report.

### GeoPT32

Webb, P.C., Thompson, M., Potts, P.J and Webber, E. (2013)  
GeoPT32 - an international proficiency test for analytical geochemistry laboratories - report on round 32 / January 2013 (Woodstock Basalt, WG-1). International Association of Geoanalysts: Unpublished report.

### GeoPT33

Webb, P.C., Thompson, M., Potts, P.J., Prusisz, B., and Young, K. (2013)  
GeoPT33 - an international proficiency test for analytical geochemistry laboratories - report on round 33 / July-August 2013 (Ball Clay, DBC-1). International Association of Geoanalysts: Unpublished report.

### GeoPT34

Webb, P.C., Thompson, M., Potts, P.J and Wilson, S. (2014)  
GeoPT34 - an international proficiency test for analytical geochemistry laboratories - report on round 34 (Granite, GRI-1) / January 2014. International Association of Geoanalysts: Unpublished report.

### GeoPT35

Webb, P.C., Thompson, M., Potts, P.J and Wilson, S. (2014)  
GeoPT35 - an international proficiency test for analytical geochemistry laboratories - report on round 35 (Tonalite, TLM-1) / August 2014. International Association of Geoanalysts: Unpublished report.

### GeoPT35A

Webb, P.C., Thompson, M., Potts, P.J and Wilson, S. (2014)  
GeoPT35A - an international proficiency test for analytical geochemistry laboratories - report on round 35A (Metalliferous sediment, SdAR-H1) / August 2014. International Association of Geoanalysts: Unpublished report.

### GeoPT36

Webb, P.C., Thompson, M., Potts, P.J and Wilson, S. (2015)  
GeoPT36 - an international proficiency test for analytical geochemistry laboratories - report on round 36 (Gabbro, GSM-1) / January 2015. International Association of Geoanalysts: Unpublished report.

### GeoPT36A

Webb, P.C., Thompson, M., Potts, P.J and Wilson, S. (2015)  
GeoPT36A - an international proficiency test for analytical geochemistry laboratories - report on round 36A (Metal-rich sediment, SdAR-M2) / January 2015. International Association of Geoanalysts: Unpublished report.

### GeoPT37

Webb, P.C., Thompson, M., Potts, P.J, Gowing, C.J.B. and Burnham, M. (2015)  
GeoPT37 - an international proficiency test for analytical geochemistry laboratories - report on round 37 (Rhyolite, ORPT-1) / July 2015. International Association of Geoanalysts: Unpublished report.

### GeoPT37A

Webb, P.C., Thompson, M., Potts, P.J, Gowing, C.J.B. and Wilson, S. (2015)  
GeoPT37A - an international proficiency test for analytical geochemistry laboratories - report on round 37A (Blended sediment, SdAR-L2) / July 2015. International Association of Geoanalysts: Unpublished report.

### GeoPT38

Webb, P.C., Thompson, M., Potts, P.J, Gowing, C.J.B. and Wilson, S.A. (2016)  
GeoPT38 - an international proficiency test for analytical geochemistry laboratories - report on round 38 (Gabbro, OU-7) / January 2016. International Association of Geoanalysts: Unpublished report.

### GeoPT38A

Webb, P.C., Thompson, M., Potts, P.J, Gowing, C.J.B. and Meisel, T. (2016)  
GeoPT38A - an international proficiency test for analytical geochemistry laboratories – special report on round 38A (Modified harzburgite, HARZ01) / June 2016. International Association of Geoanalysts: Unpublished report.

### GeoPT39

Webb, P.C., Thompson, M., Potts, P.J, Gowing, C.J.B. and Wilson, S.A. (2016)  
GeoPT39 - an international proficiency test for analytical geochemistry laboratories - report on round 39 (Syenite, SyMP-1) / July 2016. International Association of Geoanalysts: Unpublished report.

### GeoPT39A

Webb, P.C., Thompson, M., Potts, P.J, and Gowing, C.J.B. (2016)  
GeoPT39A - an international proficiency test for analytical geochemistry laboratories - report on round 39A (Nepheline syenite, MNS-1) / July 2016. International Association of Geoanalysts: Unpublished report.

### GeoPT40

Webb, P.C., Thompson, M., Potts, P.J, Gowing, C.J.B. and Wilson, S.A. (2017)  
GeoPT40 - an international proficiency test for analytical geochemistry laboratories - report on round 40 (Silty marine shale, ShWYO-1) / January 2017. International Association of Geoanalysts: Unpublished report.

### GeoPT40A

Webb, P.C., Thompson, M., Potts, P.J, Gowing, C.J.B. and Wilson, S.A. (2017)  
GeoPT40A - an international proficiency test for analytical geochemistry laboratories - report on round 40A (Calcareous organic-rich shale, ShTX-1) / January 2017. International Association of Geoanalysts: Unpublished report.

### GeoPT41

Webb, P.C., Thompson, M., Potts, P.J, Gowing, C.J.B. and Wilson, S.A. (2017)  
GeoPT41 - an international proficiency test for analytical geochemistry laboratories - report on round 41 (Andesite, ORA-1) / July 2017. International Association of Geoanalysts: Unpublished report.

### GeoPT41A

Webb, P.C., Thompson, M., Potts, P.J, Gowing, C.J.B. and Wilson, S.A. (2017)  
GeoPT41A - an international proficiency test for analytical geochemistry laboratories - report on round 41A (Mineralized stream sediment, SSCO-1) / July 2017. International Association of Geoanalysts: Unpublished report.

### GeoPT42

Webb, P.C., Thompson, M., Potts, P.J, Gowing, C.J.B. and Burnham, M. (2018)  
GeoPT42 – an international proficiency test for analytical geochemistry laboratories – report on round 42 (Queenston shale, QS-1) / January 2018. International Association of Geoanalysts: Unpublished report.

## **Appendix 1 (Cont'd)**

### **GeoPT43**

Webb, P.C., Potts, P.J., Thompson, M. and Gowing, C.J.B. (2018) GeoPT43 – an international proficiency test for analytical geochemistry laboratories – report on round 43 (Dolerite, ADS-1) / July 2018. International Association of Geoanalysts: Unpublished report.

### **GeoPT44**

Webb, P.C., Potts, P.J., Thompson, M., Gowing, C.J.B. (2019) GeoPT44 – an international proficiency test for analytical geochemistry laboratories – report on round 44 (Calcareous shale, ShCX-1) / January 2019. International Association of Geoanalysts: Unpublished report.

### **GeoPT44A**

Webb, P.C., Potts, P.J., Thompson, M. Gowing, C.J.B. and Wilson, S.A. (2019) GeoPT44A – an international proficiency test for analytical geochemistry laboratories – report on round 44A (Calcareous mudrock, CM-1) / January 2019. International Association of Geoanalysts: Unpublished report.

### **GeoPT45**

Webb, P.C., Potts, P.J., Thompson, M. Gowing, C.J.B. and Wilson, S.A. (2019) GeoPT45 – an international proficiency test for analytical geochemistry laboratories – report on round 45 (Silicified siltstone, GONV-1) / July 2019. International Association of Geoanalysts: Unpublished report.

### **GeoPT46**

Webb, P.C., Potts, P.J., Thompson, M., Gowing, C.J.B. (2020) GeoPT46 – an international proficiency test for analytical geochemistry laboratories – report on round 46 (Granodiorite, HG-1) / January 2020. International Association of Geoanalysts: Unpublished report.

### **GeoPT46A**

Webb, P.C., Potts, P.J., Thompson, M. Gowing, C.J.B. and Wilson, S.A. (2020) GeoPT46A – an international proficiency test for analytical geochemistry laboratories – report on round 46A (Phosphate rock, POLC-1) / January 2020. International Association of Geoanalysts: Unpublished report.

Table 1 - GeoPT47A Contributed data for Silty soil, NES-1. 20/11/2020

Lab Code	J1	J2	J3	J4	J5	J6	J9	J11	J12	J14	J15	J16	J18
SiO2	g 100g <sup>-1</sup>	<b>62.92</b>	80.15	78.7	79.1		78.984	80.16	78.74	80.44	80.27	80.1	82.9
TiO2	g 100g <sup>-1</sup>	<b>1.11</b>	<u>0.696</u>	0.67	0.71	0.45		0.694	0.66	0.659	0.72	0.68	0.667
Al2O3	g 100g <sup>-1</sup>	<b>13.56</b>	<u>5.758</u>	5.54	5.64	5.42		5.604	5.48	5.61	5.71	5.56	5.694
Fe2O3T	g 100g <sup>-1</sup>	<b>8.99</b>	<u>3.103</u>	2.94	3.223	3.08		3.066	3.05	3.12	3.1	3.15	3.101
Fe(II)O	g 100g <sup>-1</sup>					2.34							2.64
MnO	g 100g <sup>-1</sup>	<b>0.18</b>	<u>0.092</u>	0.091	0.089	0.095		0.091	0.09	0.090	0.091	0.09	0.090
MgO	g 100g <sup>-1</sup>	<b>1.23</b>	<u>0.466</u>	0.5	<u>0.501</u>	0.56		0.5	0.45	0.504	0.47	0.51	0.514
CaO	g 100g <sup>-1</sup>	<b>0.75</b>	<u>0.321</u>	0.32	0.3	0.8		0.31	0.32	0.224	0.31	0.32	0.325
Na2O	g 100g <sup>-1</sup>		<u>0.227</u>	0.28	<u>0.294</u>	0.1		0.336	0.27	0.274	0.28	0.34	0.293
K2O	g 100g <sup>-1</sup>	<b>4.05</b>	<u>1.034</u>	1.03	<u>1.052</u>	0.85		1.047	1.03	1.19	1.06	1.07	1.02
P2O5	g 100g <sup>-1</sup>		<u>0.234</u>	0.23	<u>0.203</u>	0.22		0.228	0.23	0.233	0.23	<u>0.23</u>	<u>0.226</u>
H2O+	g 100g <sup>-1</sup>												
CO2	g 100g <sup>-1</sup>												
LOI	g 100g <sup>-1</sup>	<b>7.1</b>	<u>7.74</u>			8.84		9	8.06	8.9	7.56	7.63	<u>7.434</u>
Ag	mg kg <sup>-1</sup>					<u>0.13</u>	0.21	0.144					
As	mg kg <sup>-1</sup>					<u>8.89</u>		11.23		13.6		10	<u>12</u>
Au	mg kg <sup>-1</sup>	<b>0.01</b>											
B	mg kg <sup>-1</sup>					<u>55.2</u>							
Ba	mg kg <sup>-1</sup>		<u>161</u>		<u>166.4</u>	180	166.270	176	11894	162.958	144	<u>159</u>	104.8
Be	mg kg <sup>-1</sup>		<u>0.92</u>		<u>1.269</u>	0.73	0.91			0.692			
Bi	mg kg <sup>-1</sup>		<u>0.13</u>		<u>0.112</u>	0.119	0.27				1		
Br	mg kg <sup>-1</sup>								14		15		
C(org)	mg kg <sup>-1</sup>												30400
C(tot)	mg kg <sup>-1</sup>												24300
Cd	mg kg <sup>-1</sup>		<u>0.42</u>		<u>0.315</u>	0.18	0.358		2.6	0.289			
Ce	mg kg <sup>-1</sup>		<u>42.3</u>		<u>46.19</u>	47.96	43.112		44.3	43.788	39	<u>43</u>	38.818
Cl	mg kg <sup>-1</sup>												
Co	mg kg <sup>-1</sup>		<u>8.37</u>		<u>8.324</u>	9.65	9.06			8.513	9		
Cr	mg kg <sup>-1</sup>		<u>45.5</u>		<u>59.27</u>	56	38.94	59	61.9		59	<u>65</u>	60.22
Cs	mg kg <sup>-1</sup>		<u>2.82</u>		<u>2.757</u>		3.25		18.1	2.67	2		2.619
Cu	mg kg <sup>-1</sup>		<u>20.9</u>		<u>17.03</u>	18.7	18.12	26	15.3	17.338	16	<u>15</u>	112.477
Dy	mg kg <sup>-1</sup>		<u>2.06</u>		<u>3.396</u>	2.63	3.172			2.733			2.881
Er	mg kg <sup>-1</sup>		<u>1.28</u>		<u>1.965</u>	1.78	1.967			1.656			
Eu	mg kg <sup>-1</sup>		<u>0.62</u>		<u>0.791</u>	0.43	0.571			0.676			
F	mg kg <sup>-1</sup>						0.034		<u>1451</u>				
Ga	mg kg <sup>-1</sup>		<u>10.7</u>		<u>7.37</u>	8.49	8.21	7	10.6		7	<u>8</u>	
Gd	mg kg <sup>-1</sup>		<u>2.76</u>		<u>3.073</u>	2.72	2.962			2.817			
Ge	mg kg <sup>-1</sup>		<u>0.78</u>				0.13						
Hf	mg kg <sup>-1</sup>		<u>2.72</u>		<u>8.246</u>		2.123			4.467	8		
Hg	mg kg <sup>-1</sup>												
Ho	mg kg <sup>-1</sup>		<u>0.4</u>		<u>0.603</u>	0.51	0.598			0.563			
I	mg kg <sup>-1</sup>								11.2		5.2		
In	mg kg <sup>-1</sup>					<u>0.069</u>	0.024						
La	mg kg <sup>-1</sup>		<u>21.9</u>		<u>24.33</u>	23.45	24.814		17	22.779	21	<u>24</u>	19.539
Li	mg kg <sup>-1</sup>		<u>23.3</u>		<u>20.21</u>		22.35			22.12			
Lu	mg kg <sup>-1</sup>		<u>0.19</u>		<u>0.241</u>	0.31	0.308			0.248			
Mo	mg kg <sup>-1</sup>		<u>0.63</u>		<u>0.676</u>	1.4	0.55						
N	mg kg <sup>-1</sup>												
Nb	mg kg <sup>-1</sup>		<u>11.8</u>		<u>14.23</u>		9.9		14.5	16.663	14	<u>15</u>	
Nd	mg kg <sup>-1</sup>		<u>18</u>		<u>19.74</u>	19.4	19.243		20.2	19.014	16		16.78
Ni	mg kg <sup>-1</sup>		<u>20.4</u>		<u>17.87</u>	21.18	18.4		16.7	19.097	17	<u>18</u>	20.58
Pb	mg kg <sup>-1</sup>		<u>25.6</u>		<u>22.82</u>	14	26.58		25.4	22.998	24	<u>26</u>	
Pr	mg kg <sup>-1</sup>		<u>5.02</u>		<u>5.159</u>	5.22	4.961			5.139			5.586
Rb	mg kg <sup>-1</sup>		<u>52.9</u>		<u>55.6</u>	54.36	58.53	58	47.7	52.639	52	<u>56</u>	46.982
Re	mg kg <sup>-1</sup>												
S	mg kg <sup>-1</sup>					<u>442.7</u>	400		425				385
Sb	mg kg <sup>-1</sup>		<u>1.12</u>		<u>1.083</u>	0.15	1.21				0.9		
Sc	mg kg <sup>-1</sup>		<u>5.78</u>			5.4	6.13		4.1	5.577	4	<u>7</u>	
Se	mg kg <sup>-1</sup>					<u>0.485</u>	0.77	2.7			1		
Sm	mg kg <sup>-1</sup>		<u>3.14</u>		<u>3.216</u>	3.13	3.578	3		3.332	4		
Sn	mg kg <sup>-1</sup>		<u>1.21</u>		<u>1.765</u>		2		6.8	2.201	2.2		
Sr	mg kg <sup>-1</sup>		<u>27.1</u>		<u>24.85</u>	29.7	27.53	25	29.1	27.592	26	<u>28</u>	31.84
Ta	mg kg <sup>-1</sup>		<u>0.78</u>		<u>0.911</u>		1.34			1.013	2		
Tb	mg kg <sup>-1</sup>		<u>0.37</u>		<u>0.446</u>	0.26	0.451			0.443			
Te	mg kg <sup>-1</sup>						0.029	0.14	2.8				
Th	mg kg <sup>-1</sup>		<u>5.51</u>		<u>13.77</u>	5.05	5.77		7.4	5.679	5	<u>6</u>	
Tl	mg kg <sup>-1</sup>		<u>0.3</u>		<u>0.315</u>	0.33	0.359			0.317			0.361
Tm	mg kg <sup>-1</sup>		<u>0.19</u>		<u>0.256</u>	0.24	0.316			0.24			
U	mg kg <sup>-1</sup>		<u>1.89</u>		<u>5.231</u>	2.36	1.89			2.054	3	<u>3</u>	1.963
V	mg kg <sup>-1</sup>		<u>48</u>		<u>47.65</u>	53.4	47.17	64	47.6	51.138	48	<u>52</u>	59.86
W	mg kg <sup>-1</sup>		<u>0.83</u>		<u>1.008</u>		0.52			1.042	3		
Y	mg kg <sup>-1</sup>		<u>12</u>		<u>18.67</u>	16.5	16.944		17.1	16.327	16	<u>18</u>	8.505
Yb	mg kg <sup>-1</sup>		<u>1.28</u>		<u>2.068</u>	1.66	1.751			1.613	2		
Zn	mg kg <sup>-1</sup>		<u>63.4</u>		<u>65.4</u>	63	60.45	64	48.9	63.894	62	<u>63</u>	60.72
Zr	mg kg <sup>-1</sup>		<u>99.3</u>		<u>287.9</u>	242	75.12	288	306.7	165.587	323	<u>333</u>	<u>316</u>

Bold entries are Data Quality 1 - Underlined entries are Data Quality 2

Table 1 - GeoPT47A Contributed data for Silty soil, NES-1. 20/11/2020

Lab Code	J20	J21	J22	J24	J25	J26	J27	J28	J29	J30	J31	J33	J34	
SiO <sub>2</sub>	g 100g <sup>-1</sup>	<b>79.39</b>	79.9	<b>78.14</b>	<u>80.126</u>	<b>80.39</b>	<u>77.57</u>	<b>81.84</b>		<u>79.83</u>	<b>79.453</b>	<u>80.229</u>	<b>79.2</b>	<b>79.9</b>
TiO <sub>2</sub>	g 100g <sup>-1</sup>	<b>0.69</b>	<u>0.689</u>	<b>0.678</b>	<u>0.690</u>	<b>0.67</b>	<u>0.67</u>	<b>0.73</b>	<u>0.67</u>	<b>0.7</b>	<u>0.672</u>	<b>0.683</b>	<b>0.72</b>	<b>0.694</b>
Al <sub>2</sub> O <sub>3</sub>	g 100g <sup>-1</sup>	<b>5.61</b>	5.67	<b>5.59</b>	<u>5.739</u>	<b>5.68</b>	<u>5.55</u>	<b>5.68</b>	<b>5.7</b>	<b>5.2</b>	<u>5.548</u>	<b>5.701</b>	<b>5.59</b>	<b>5.698</b>
Fe <sub>2</sub> O <sub>3</sub> T	g 100g <sup>-1</sup>	<b>3.24</b>	3.18	<b>3.101</b>	<u>3.161</u>	<b>3.1</b>	<u>3.04</u>	<b>3.15</b>	<u>3.07</u>	<u>3.29</u>	<b>3.1</b>	<u>3.049</u>	<b>3.35</b>	<b>3.036</b>
Fe(II)O	g 100g <sup>-1</sup>	<b>2.373</b>			<u>2.398</u>			<b>0.16</b>						
MnO	g 100g <sup>-1</sup>	<b>0.09</b>	<u>0.092</u>	<b>0.090</b>	<u>0.093</u>	<b>0.09</b>	<u>0.09</u>	<b>0.09</b>	<u>0.09</u>	<b>0.1</b>	<u>0.115</u>	<b>0.089</b>	<b>0.098</b>	<b>0.092</b>
MgO	g 100g <sup>-1</sup>	<b>0.49</b>	0.49	<b>0.48</b>	<u>0.538</u>	<b>0.49</b>	<u>0.5</u>	<b>0.47</b>	<b>0.5</b>	<u>0.49</u>	<u>0.515</u>	<b>0.52</b>	<b>0.51</b>	<b>0.534</b>
CaO	g 100g <sup>-1</sup>	<b>0.32</b>	0.32	<b>0.32</b>	<u>0.317</u>	<b>0.31</b>	<u>0.58</u>	<b>0.31</b>	<u>3.06</u>	<b>0.3</b>	<u>0.215</u>	<b>0.302</b>	<b>0.37</b>	<b>0.337</b>
Na <sub>2</sub> O	g 100g <sup>-1</sup>	<b>0.28</b>	0.28	<b>0.31</b>	<u>0.335</u>	<b>0.28</b>	<u>0.31</u>	<b>0.13</b>	<u>0.29</u>	<b>0.27</b>	<u>0.256</u>	<b>0.289</b>	<b>0.28</b>	<b>0.339</b>
K <sub>2</sub> O	g 100g <sup>-1</sup>	<b>0.97</b>	1.05	<b>1.02</b>	<u>1.071</u>	<b>1.03</b>	<u>1.06</u>	<b>1.05</b>	<b>1.01</b>	<u>1.09</u>	<u>1.06</u>	<u>1.053</u>	<b>1.05</b>	<b>1.04</b>
P <sub>2</sub> O <sub>5</sub>	g 100g <sup>-1</sup>	<b>0.23</b>	<u>0.229</u>	<b>0.224</b>	<u>0.233</u>	<b>0.23</b>	<u>0.22</u>	<b>0.23</b>	<u>0.22</u>	<u>0.22</u>	<u>0.229</u>	<u>0.342</u>	<u>0.237</u>	<u>0.223</u>
H <sub>2</sub> O+	g 100g <sup>-1</sup>	<b>2.750</b>			<u>3.81</u>			<b>4.62</b>		<u>1.24</u>				
CO <sub>2</sub>	g 100g <sup>-1</sup>	<b>10.702</b>					<u>10.3</u>							<b>0.62</b>
LOI	g 100g <sup>-1</sup>	<b>7.58</b>	7.87	<b>8.41</b>	<u>7.406</u>	<b>7.47</b>	<u>9.44</u>			<u>8.44</u>	<u>7.757</u>	<b>7.76</b>	<b>7.88</b>	<b>8.034</b>
Ag	mg kg <sup>-1</sup>	<b>0.148</b>			<u>0.16</u>	<u>0.099</u>	<u>0.101</u>	<u>0.21</u>						
As	mg kg <sup>-1</sup>	<b>10.2</b>			<u>10.2</u>	<u>9.232</u>					<u>12</u>		<b>7.1</b>	
Au	mg kg <sup>-1</sup>													
B	mg kg <sup>-1</sup>	<b>32.387</b>												
Ba	mg kg <sup>-1</sup>	<b>154</b>	<u>158</u>	<b>157</b>	<u>163.260</u>	<b>165.329</b>	<u>160.830</u>	<b>158</b>	<b>159</b>		<u>174</u>	<u>215</u>	<b>187</b>	<b>167.3</b>
Be	mg kg <sup>-1</sup>	<b>0.71</b>			<u>0.72</u>	<u>0.731</u>	<b>0.936</b>			<b>0.8</b>				
Bi	mg kg <sup>-1</sup>	<b>0.13</b>				<u>0.17</u>	<b>0.133</b>			<b>0.15</b>				
Br	mg kg <sup>-1</sup>												<u>13</u>	
C(org)	mg kg <sup>-1</sup>	<b>14752</b>		<u>24450</u>				<u>29600</u>						<b>23300</b>
C(tot)	mg kg <sup>-1</sup>			<u>26000</u>	<u>27928</u>		<u>28090.300</u>					<u>29748</u>		<b>29500</b>
Cd	mg kg <sup>-1</sup>	<b>0.27</b>			<u>0.301</u>	<u>0.24</u>	<b>0.243</b>			<b>0.15</b>				
Ce	mg kg <sup>-1</sup>	<b>42.4</b>	<u>43.63</u>	<b>46.9</b>	<u>42.749</u>	<b>40.759</b>	<u>42.93</u>	<b>48</b>	<b>43.6</b>		<u>47</u>		<b>41</b>	
Cl	mg kg <sup>-1</sup>	<b>59.739</b>						<u>25</u>						
Co	mg kg <sup>-1</sup>	<b>8.34</b>			<u>8.87</u>	<u>8.675</u>	<b>8.385</b>	<u>8.63</u>	<b>8</b>	<b>8.42</b>				<b>7.5</b>
Cr	mg kg <sup>-1</sup>	<b>69.3</b>	<b>63</b>	<b>75.7</b>	<u>59.77</u>	<b>64.744</b>	<u>65.24</u>	<b>72</b>	<b>62</b>		<u>66</u>	<u>70</u>	<b>61</b>	<b>71.5</b>
Cs	mg kg <sup>-1</sup>	<b>2.68</b>	<u>2.59</u>		<u>2.783</u>	<b>2.57</b>	<u>3.26</u>	<b>7</b>	<b>2.64</b>					
Cu	mg kg <sup>-1</sup>	<b>20.2</b>	<b>19</b>	<b>18.5</b>	<u>18.59</u>	<b>19.009</b>	<u>17.38</u>	<b>22</b>	<b>17.6</b>		<u>12</u>		<b>17</b>	<b>15.8</b>
Dy	mg kg <sup>-1</sup>	<b>2.97</b>	<u>3.22</u>	<u>3.201</u>	<u>2.892</u>	<b>2.953</b>	<u>2.87</u>		<b>3</b>					
Er	mg kg <sup>-1</sup>	<b>1.77</b>	<u>1.91</u>	<b>1.901</b>	<u>1.795</u>	<b>1.835</b>	<u>1.7</u>		<b>1.88</b>					
Eu	mg kg <sup>-1</sup>	<b>0.679</b>	<u>0.73</u>	<b>0.68</b>	<u>0.663</u>	<b>0.694</b>	<u>0.64</u>		<b>0.68</b>					
F	mg kg <sup>-1</sup>	<b>277</b>		<u>300</u>			<u>230</u>							
Ga	mg kg <sup>-1</sup>	<b>8.32</b>	<b>8</b>		<u>8.044</u>	<b>7.955</b>	<u>8.01</u>	<b>11</b>	<b>8.1</b>		<u>9</u>		<b>7.9</b>	
Gd	mg kg <sup>-1</sup>	<b>2.87</b>	<u>3.01</u>	<u>3.501</u>	<u>2.829</u>	<b>2.88</b>	<u>3.04</u>		<b>2.88</b>					
Ge	mg kg <sup>-1</sup>	<b>1.29</b>												
Hf	mg kg <sup>-1</sup>	<b>8.19</b>	<u>7.57</u>	<b>8.85</b>	<u>5.55</u>	<b>6.633</b>	<u>8.09</u>	<b>4</b>	<b>8.07</b>		<u>7</u>		<b>12</b>	
Hg	mg kg <sup>-1</sup>	<b>0.084</b>												
Ho	mg kg <sup>-1</sup>	<b>0.643</b>	<b>0.68</b>	<b>0.65</b>	<u>0.597</u>	<b>0.621</b>	<u>0.61</u>		<b>0.62</b>					
I	mg kg <sup>-1</sup>													
In	mg kg <sup>-1</sup>				<u>0.026</u>									
La	mg kg <sup>-1</sup>	<b>22</b>	<u>22.92</u>	<b>24.6</b>	<u>22.5</u>	<b>20.241</b>	<u>22.14</u>	<b>28</b>	<b>22.8</b>	<u>211</u>	<u>26</u>		<b>13</b>	
Li	mg kg <sup>-1</sup>	<b>21.849</b>			<u>23.2</u>	<u>21.21</u>	<u>20.995</u>			<b>21.3</b>				
Lu	mg kg <sup>-1</sup>	<b>0.287</b>	<u>0.28</u>	<b>0.31</b>	<u>0.267</u>	<b>0.28</b>	<u>0.25</u>			<b>0.29</b>				
Mo	mg kg <sup>-1</sup>	<b>0.85</b>			<u>0.56</u>	<b>0.7</b>	<u>0.746</u>	<u>1.09</u>	<b>2</b>	<b>0.7</b>				
N	mg kg <sup>-1</sup>													
Nb	mg kg <sup>-1</sup>	<b>12.5</b>	<b>13.82</b>	<b>14.6</b>	<u>14.535</u>	<b>13.283</b>	<u>14.26</u>	<b>18</b>	<b>14.8</b>		<u>18</u>		<b>13</b>	
Nd	mg kg <sup>-1</sup>	<b>18.3</b>	<b>18.74</b>	<b>19.4</b>	<u>17.853</u>	<b>18.035</b>	<u>17.69</u>	<b>20</b>	<b>18.3</b>	<u>182</u>	<u>16</u>		<b>19</b>	
Ni	mg kg <sup>-1</sup>	<b>20</b>	<b>15</b>	<b>20.6</b>	<u>20.42</u>	<b>18.437</b>	<u>25.75</u>	<b>28</b>	<b>19.3</b>		<u>17</u>		<b>19</b>	<b>22.1</b>
Pb	mg kg <sup>-1</sup>	<b>24.5</b>	<b>23.66</b>	<b>24.8</b>	<u>24.183</u>	<b>25.253</b>		<b>40</b>	<b>26.3</b>		<u>28</u>	<u>41</u>		<b>35.9</b>
Pr	mg kg <sup>-1</sup>	<b>4.92</b>	<b>5.09</b>	<b>4.96</b>	<u>4.951</u>	<b>4.893</b>	<u>4.73</u>			<b>5.02</b>				
Rb	mg kg <sup>-1</sup>	<b>54.6</b>	<b>52.2</b>	<b>76.1</b>	<u>56.035</u>	<b>47.602</b>	<u>57.43</u>	<b>63</b>	<b>54</b>		<u>48</u>	<u>52</u>	<b>52</b>	
Re	mg kg <sup>-1</sup>													
S	mg kg <sup>-1</sup>	<b>405</b>		<u>500</u>	<u>458</u>		<u>431.8</u>	<u>590</u>				<u>446</u>		
Sb	mg kg <sup>-1</sup>	<b>1.28</b>		<u>1.06</u>	<u>1.377</u>	<b>1.197</b>	<u>1.27</u>							
Sc	mg kg <sup>-1</sup>	<b>5.55</b>	<b>5.2</b>	<b>5.16</b>	<u>5.68</u>	<b>5.318</b>	<u>5.3</u>	<b>9</b>	<b>5.54</b>				<b>6.5</b>	
Se	mg kg <sup>-1</sup>				<b>1.26</b>									
Sm	mg kg <sup>-1</sup>	<b>3.29</b>	<b>3.49</b>	<b>3.54</b>	<u>3.17</u>	<b>3.328</b>	<u>3.2</u>			<b>3.41</b>				
Sn	mg kg <sup>-1</sup>	<b>2.27</b>				<u>1.94</u>	<b>1.815</b>		<b>3</b>	<b>2.21</b>		<u>2</u>		
Sr	mg kg <sup>-1</sup>	<b>26.8</b>	<b>28</b>	<b>27.3</b>	<u>29.05</u>	<b>25.1</b>	<u>28.04</u>	<b>34</b>	<b>25.9</b>			<u>27</u>	<b>25</b>	
Ta	mg kg <sup>-1</sup>	<b>1.07</b>	<b>0.96</b>	<b>0.85</b>	<u>0.900</u>	<b>0.865</b>	<u>0.87</u>	<b>7</b>	<b>0.98</b>					
Tb	mg kg <sup>-1</sup>	<b>0.455</b>	<b>0.52</b>	<b>0.47</b>	<u>0.454</u>	<b>0.484</b>	<u>0.47</u>			<b>0.48</b>				
Te	mg kg <sup>-1</sup>						<b>0.024</b>							
Th	mg kg <sup>-1</sup>	<b>5.82</b>	<b>5.89</b>	<b>6.301</b>	<u>5.550</u>	<b>5.769</b>	<u>5.81</u>	<b>12</b>	<b>6.24</b>		<u>7</u>			
Tl	mg kg <sup>-1</sup>					<b>0.33</b>	<u>0.291</u>			<b>0.36</b>				
Tm	mg kg <sup>-1</sup>	<b>0.278</b>	<b>0.28</b>	<b>0.28</b>	<u>0.255</u>	<b>0.28</b>	<u>0.25</u>			<b>0.29</b>				
U	mg kg <sup>-1</sup>	<b>2.09</b>	<b>2.07</b>	<b>2.201</b>	<u>1.978</u>	<b>2.144</b>	<u>2.1</u>	<b>3</b>	<b>2.38</b>				<b>2.2</b>	
V	mg kg <sup>-1</sup>	<b>46.3</b>	<b>51</b>	<b>61.4</b>	<u>54.08</u>	<b>44.956</b>	<u>50.42</u>	<b>49</b>	<b>46</b>	<u>128</u>	<u>69</u>	<b>51</b>	<b>104.3</b>	
W	mg kg <sup>-1</sup>	<b>1.15</b>				<u>1.06</u>	<b>1.071</b>		<b>2</b>	<b>1.04</b>				
Y	mg kg <sup>-1</sup>	<b>17.5</b>	<b>18.37</b>	<b>18.01</b>	<u>18.608</u>	<b>17.552</b>	<u>17.57</u>	<b>21</b>	<b>19.1</b>		<u>24</u>	<u>14</u>	<b>17</b>	
Yb	mg kg <sup>-1</sup>	<b>1.86</b>	<b>1.81</b>	<b>2.001</b>	<u>1.738</u>	<b>1.82</b>	<u>1.66</u>			<b>1.91</b>				
Zn	mg kg <sup>-1</sup>	<b>67.9</b>	<b>66</b>	<b>63.8</b>	<u>64.71</u>	<b>61.624</b>	<u>68.05</u>	<b>74</b>	<b>63.3</b>		<u>65</u>	<u>72</u>	<b>58</b>	<b>77.2</b>
Zr	mg kg <sup>-1</sup>	<b>326</b>	<b>300</b>	<b>362</b>	<u>245</u>	<b>311.422</b>	<u>302.280</u>	<b>332</b>	<b>348</b>		<u>369</u>	<u>326</u>	<b>321</b>	<b>345.4</b>

Bold entries are Data Quality 1 - Underlined entries are Data Quality 2

Table 1 - GeoPT47A Contributed data for Silty soil, NES-1. 20/11/2020

Lab Code	J36	J37	J39	J40	J41	J42	J43	J45	J46	J49	J52	J54	J55	
SiO <sub>2</sub>	g 100g <sup>-1</sup>	<b>80.401</b>	81.55	78.66	79.71	79.85	79.994	80.18	77.83	<b>79</b>	77.02	79.1	79.3	80.29
TiO <sub>2</sub>	g 100g <sup>-1</sup>	<b>0.72</b>	<u>0.692</u>	<u>0.614</u>	<u>0.736</u>	<u>0.7</u>	<u>0.714</u>	<u>0.7</u>	<u>0.68</u>	<u>0.73</u>	<u>0.702</u>	<u>0.51</u>	<u>0.71</u>	<u>0.71</u>
Al <sub>2</sub> O <sub>3</sub>	g 100g <sup>-1</sup>	<b>5.664</b>	<u>5.82</u>	<u>5.561</u>	<u>5.77</u>	<u>5.57</u>	<u>5.688</u>	<u>5.81</u>	<u>5.59</u>	<u>5.56</u>	<u>5.77</u>	<u>5.76</u>	<u>5.53</u>	<u>5.81</u>
Fe <sub>2</sub> O <sub>3</sub> T	g 100g <sup>-1</sup>	<b>3.161</b>	<u>3.19</u>	<u>3.127</u>	<u>3.305</u>	<u>3.03</u>	<u>3.217</u>	<u>3.33</u>	<u>3.07</u>	<u>3.27</u>	<u>3.46</u>	<u>2.76</u>	<u>3.06</u>	<u>3.17</u>
Fe(II)O	g 100g <sup>-1</sup>													
MnO	g 100g <sup>-1</sup>	<b>0.096</b>	<u>0.098</u>	<u>0.087</u>	<u>0.100</u>	<u>0.08</u>	<u>0.094</u>	<u>0.070</u>	<u>0.09</u>	<u>0.11</u>	<u>0.102</u>	<u>0.093</u>	<u>0.1</u>	<u>0.09</u>
MgO	g 100g <sup>-1</sup>	<b>0.477</b>	<u>0.43</u>	<u>0.495</u>	<u>0.525</u>	<u>0.49</u>	<u>0.489</u>	<u>0.57</u>	<u>0.5</u>	<u>0.71</u>	<u>0.674</u>	<u>0.42</u>	<u>0.51</u>	<u>0.49</u>
CaO	g 100g <sup>-1</sup>	<b>0.32</b>	<u>0.34</u>	<u>0.298</u>	<u>0.327</u>	<u>0.33</u>	<u>0.328</u>	<u>0.33</u>	<u>0.31</u>	<u>0.88</u>	<u>0.373</u>	<u>0.28</u>	<u>0.33</u>	<u>0.35</u>
Na <sub>2</sub> O	g 100g <sup>-1</sup>	<b>0.162</b>	<u>0.27</u>	<u>0.287</u>	<u>0.349</u>	<u>0.16</u>	<u>0.277</u>	<u>0.32</u>	<u>0.31</u>	<u>0.39</u>	<u>0.291</u>	<u>0.34</u>	<u>0.24</u>	<u>0.28</u>
K <sub>2</sub> O	g 100g <sup>-1</sup>	<b>1.045</b>	<u>1.14</u>	<u>1.035</u>	<u>1.028</u>	<u>0.98</u>	<u>1.025</u>	<u>1.03</u>	<u>1.09</u>	<u>1.06</u>	<u>1.18</u>	<u>0.92</u>	<u>1.05</u>	<u>1.03</u>
P <sub>2</sub> O <sub>5</sub>	g 100g <sup>-1</sup>	<b>0.198</b>	<u>0.23</u>	<u>0.229</u>	<u>0.237</u>	<u>0.222</u>	<u>0.232</u>	<u>0.249</u>	<u>0.225</u>		<u>0.373</u>		<u>0.23</u>	<u>0.22</u>
H <sub>2</sub> O+	g 100g <sup>-1</sup>													
CO <sub>2</sub>	g 100g <sup>-1</sup>													
LOI	g 100g <sup>-1</sup>	<b>7.65</b>	<u>7.63</u>		7.68	<u>8.39</u>	<u>7.54</u>	<u>7.47</u>	<u>9.11</u>	<u>8.14</u>		<u>7.66</u>	<u>8.29</u>	<u>7.3</u>
Ag	mg kg <sup>-1</sup>													
As	mg kg <sup>-1</sup>				14		<u>7.67</u>	<u>9.9</u>				<u>12</u>	<u>13.8</u>	
Au	mg kg <sup>-1</sup>													
B	mg kg <sup>-1</sup>	<u>33.27</u>												
Ba	mg kg <sup>-1</sup>	<b>176.3</b>		<u>159.1</u>	162		156.3	<u>141.8</u>			<u>319</u>		<u>186</u>	<u>152</u>
Be	mg kg <sup>-1</sup>						<u>0.73</u>							
Bi	mg kg <sup>-1</sup>													
Br	mg kg <sup>-1</sup>							<u>14.1</u>						
C(org)	mg kg <sup>-1</sup>						28000							
C(tot)	mg kg <sup>-1</sup>			28600				30300			27500			2.86
Cd	mg kg <sup>-1</sup>													
Ce	mg kg <sup>-1</sup>	<b>34.6</b>			49		<u>43.16</u>	<u>33.8</u>		41.6			<u>48</u>	
Cl	mg kg <sup>-1</sup>		<u>56</u>	<u>109</u>							<u>141</u>			
Co	mg kg <sup>-1</sup>	<b>12.07</b>			12		<u>8.5</u>	<u>9.9</u>					<u>9.2</u>	
Cr	mg kg <sup>-1</sup>	<b>55.7</b>		<u>39.77</u>	72		<u>64.6</u>	<u>52.7</u>			<u>77</u>		<u>55.6</u>	
Cs	mg kg <sup>-1</sup>	<b>4.36</b>					<u>2.47</u>	<u>2.6</u>					<u>3.2</u>	
Cu	mg kg <sup>-1</sup>	<b>15.3</b>			23		<u>14.8</u>	<u>17</u>			<u>103</u>		<u>12.5</u>	
Dy	mg kg <sup>-1</sup>	<u>2.18</u>					<u>3.04</u>			<u>2.37</u>				
Er	mg kg <sup>-1</sup>	<u>1.35</u>					<u>1.91</u>			<u>1.08</u>				
Eu	mg kg <sup>-1</sup>	<u>0.664</u>					<u>0.67</u>			<u>0.67</u>				
F	mg kg <sup>-1</sup>		<u>305</u>	<u>575</u>										
Ga	mg kg <sup>-1</sup>	<b>10.71</b>			9		<u>8.22</u>	<u>6.9</u>					<u>7</u>	
Gd	mg kg <sup>-1</sup>	<b>2.4</b>					<u>2.86</u>			<u>2.84</u>				
Ge	mg kg <sup>-1</sup>	<u>1.65</u>												
Hf	mg kg <sup>-1</sup>	<u>2.694</u>					<u>7.93</u>	<u>9.7</u>					<u>0.6</u>	
Hg	mg kg <sup>-1</sup>					<u>0.082</u>	<u>0.084</u>	<u>0.08</u>						
Ho	mg kg <sup>-1</sup>	<b>0.436</b>					<u>0.63</u>			<u>0.39</u>				
I	mg kg <sup>-1</sup>						<u>7.7</u>							
In	mg kg <sup>-1</sup>													
La	mg kg <sup>-1</sup>	<b>16.9</b>					<u>23.28</u>	<u>22.4</u>		<u>21.1</u>	<u>50</u>		<u>37.8</u>	
Li	mg kg <sup>-1</sup>	<b>28.43</b>					<u>98</u>							
Lu	mg kg <sup>-1</sup>	<b>0.177</b>					<u>0.29</u>			<u>0.195</u>				
Mo	mg kg <sup>-1</sup>						<u>1</u>							
N	mg kg <sup>-1</sup>												<u>0.32</u>	
Nb	mg kg <sup>-1</sup>	<b>14.69</b>			15	<u>14</u>	<u>13.03</u>	<u>13.7</u>					<u>16</u>	<u>13</u>
Nd	mg kg <sup>-1</sup>	<b>15.07</b>			18		<u>19.16</u>	<u>17.7</u>		<u>18</u>	<u>53</u>		<u>20.8</u>	
Ni	mg kg <sup>-1</sup>	<b>18.2</b>			21		<u>16.5</u>	<u>16.3</u>			<u>37</u>		<u>17</u>	
Pb	mg kg <sup>-1</sup>	<b>22.8</b>			24		<u>23.96</u>	<u>22.7</u>						<u>45.6</u>
Pr	mg kg <sup>-1</sup>	<b>3.83</b>					<u>5.2</u>			<u>4.64</u>				
Rb	mg kg <sup>-1</sup>	<b>52.7</b>			60	<u>63</u>	<u>53.68</u>	<u>50.5</u>			<u>59</u>		<u>58</u>	<u>52</u>
Re	mg kg <sup>-1</sup>													
S	mg kg <sup>-1</sup>			1028				<u>440</u>		<u>300</u>	<u>1800</u>			
Sb	mg kg <sup>-1</sup>							<u>4.4</u>						
Sc	mg kg <sup>-1</sup>	<b>11.5</b>					<u>5.1</u>	<u>3.9</u>					<u>8.6</u>	
Se	mg kg <sup>-1</sup>													
Sm	mg kg <sup>-1</sup>	<b>2.96</b>					<u>3.41</u>	<u>1.4</u>		<u>3.19</u>				<u>4.2</u>
Sn	mg kg <sup>-1</sup>						<u>1.98</u>	<u>4.7</u>						
Sr	mg kg <sup>-1</sup>	<b>31.17</b>			32	<u>34</u>	<u>26.3</u>	<u>25.5</u>			<u>35</u>		<u>32</u>	<u>26</u>
Ta	mg kg <sup>-1</sup>	<b>0.921</b>					<u>0.9</u>							
Tb	mg kg <sup>-1</sup>	<b>0.369</b>					<u>0.44</u>			<u>0.49</u>				
Te	mg kg <sup>-1</sup>							<u>3.4</u>						
Th	mg kg <sup>-1</sup>	<b>5.52</b>					<u>5.8</u>	<u>4</u>		<u>5.63</u>				<u>3.8</u>
Tl	mg kg <sup>-1</sup>						<u>0.25</u>							
Tm	mg kg <sup>-1</sup>	<b>0.183</b>					<u>0.28</u>			<u>0.26</u>				
U	mg kg <sup>-1</sup>	<b>2.43</b>					<u>2.16</u>	<u>2.4</u>		<u>2</u>			<u>2.8</u>	
V	mg kg <sup>-1</sup>	<b>54.4</b>		<u>53.69</u>	58	<u>42</u>	<u>42.5</u>	<u>40.2</u>					<u>52</u>	
W	mg kg <sup>-1</sup>							<u>1.9</u>					<u>8.7</u>	
Y	mg kg <sup>-1</sup>	<b>20</b>			19	<u>13</u>	<u>17.8</u>	<u>16.7</u>		<u>11</u>			<u>17</u>	<u>17.8</u>
Yb	mg kg <sup>-1</sup>	<b>1.43</b>					<u>1.85</u>	<u>1</u>		<u>1.14</u>				
Zn	mg kg <sup>-1</sup>	<b>63.3</b>		<u>67.61</u>	69		<u>61.9</u>	<u>57.3</u>			<u>55</u>	<u>64.79</u>	<u>64</u>	<u>61.2</u>
Zr	mg kg <sup>-1</sup>	<b>306.1</b>		<u>109.4</u>	328	<u>308</u>	<u>328.820</u>	<u>321.8</u>			<u>342</u>		<u>316</u>	<u>317</u>

Bold entries are Data Quality 1 - Underlined entries are Data Quality 2

Table 1 - GeoPT47A Contributed data for Silty soil, NES-1. 20/11/2020

Lab Code	J56	J57	J59	J60	J61	J62	J64	J65	J67	J68	J69	J70	J71
SiO2	g 100g <sup>-1</sup>	<u>80.96</u>	78.5	<u>80.01</u>	80.5	78.89	79.3	80.04	80.156	79.54	80.3		80
TiO2	g 100g <sup>-1</sup>	<u>0.71</u>	<u>0.64</u>	<u>0.71</u>	<u>0.78</u>	<u>0.76</u>	0.7	0.7	0.702	<u>0.680</u>	0.7	0.704	<u>0.639</u>
Al2O3	g 100g <sup>-1</sup>	<u>5.8</u>	<u>5.61</u>	<u>5.81</u>	<u>5.6</u>	<u>6.12</u>	5.51	5.39	5.64	<u>5.653</u>	5.7	5.476	<u>5.4</u>
Fe2O3T	g 100g <sup>-1</sup>	<u>3.12</u>	<u>3.37</u>	<u>3.13</u>	<u>3.1</u>	<u>3.64</u>	<u>3.05</u>	<u>3.17</u>	3.241	<u>3.112</u>	3.17	3.121	<u>3.05</u>
Fe(II)O	g 100g <sup>-1</sup>												1.35
MnO	g 100g <sup>-1</sup>	<u>0.11</u>	<u>0.1</u>	<u>0.08</u>	<u>0.09</u>	<u>0.09</u>	0.087	0.092	0.094	<u>0.091</u>	0.09	0.092	<u>0.087</u>
MgO	g 100g <sup>-1</sup>	<u>0.47</u>	<u>0.55</u>	<u>0.52</u>	<u>0.46</u>	<u>0.53</u>	0.484	0.41	0.486	<u>0.508</u>	0.5	0.512	<u>0.485</u>
CaO	g 100g <sup>-1</sup>	<u>0.32</u>	<u>0.37</u>	<u>0.31</u>	<u>0.32</u>	<u>0.37</u>	0.452	0.31	0.308	<u>0.324</u>	0.34	0.335	<u>0.308</u>
Na2O	g 100g <sup>-1</sup>	<u>0.37</u>	<u>0.3</u>	<u>0.34</u>	<u>0.33</u>	<u>0.31</u>	0.276	0.14	0.413	<u>0.200</u>	0.33	0.258	<u>0.23</u>
K2O	g 100g <sup>-1</sup>	<u>1.07</u>	<u>1.01</u>	<u>1.06</u>	<u>1.02</u>	<u>1.05</u>	1.053	1.04	1.06	<u>1.045</u>	1.05	1.023	<u>1.03</u>
P2O5	g 100g <sup>-1</sup>	<u>0.23</u>	<u>0.22</u>	<u>0.23</u>	<u>0.23</u>	<u>0.15</u>	0.348	0.227	0.229	<u>0.223</u>	0.24	0.226	<u>0.216</u>
H2O+	g 100g <sup>-1</sup>												4.44
CO2	g 100g <sup>-1</sup>												4.71
LOI	g 100g <sup>-1</sup>	<u>8.26</u>		<u>7.6</u>	<u>7.76</u>	<u>7.6</u>	8.6	7.53	7.52	<u>7.68</u>	7.67	8.563	<u>7.6</u>
Ag	mg kg <sup>-1</sup>									0.401	0.135		
As	mg kg <sup>-1</sup>		<u>11</u>							10.04	8.85		
Au	mg kg <sup>-1</sup>												
B	mg kg <sup>-1</sup>									15.76			
Ba	mg kg <sup>-1</sup>	<u>159</u>	<u>181</u>			<u>157</u>	160	168	159.7		190	161.720	<u>159.5</u>
Be	mg kg <sup>-1</sup>						0.722	0.699					<u>0.82</u>
Bi	mg kg <sup>-1</sup>							0.158	0.145				
Br	mg kg <sup>-1</sup>												
C(org)	mg kg <sup>-1</sup>												
C(tot)	mg kg <sup>-1</sup>										44000		
Cd	mg kg <sup>-1</sup>						0.26	0.294	0.182				
Ce	mg kg <sup>-1</sup>	<u>54</u>	<u>43</u>				43.45	44	43.974		49	42.02	<u>44.6</u>
Cl	mg kg <sup>-1</sup>												
Co	mg kg <sup>-1</sup>	<u>6</u>	<u>12</u>			<u>8</u>	8.51	8.132					8.19
Cr	mg kg <sup>-1</sup>	<u>59</u>	<u>57</u>			<u>24</u>	66.5	63	73.8		120	65.47	<u>57.27</u>
Cs	mg kg <sup>-1</sup>						2.71	2.723	2.727				2.5
Cu	mg kg <sup>-1</sup>	<u>20</u>	<u>22</u>			<u>12</u>	17.26	17.33	20.78		20	17.66	<u>17.3</u>
Dy	mg kg <sup>-1</sup>		<u>2</u>				2.89	2.186	3.055				2.91
Er	mg kg <sup>-1</sup>		<u>1.1</u>				1.81	1.791	1.884				1.71
Eu	mg kg <sup>-1</sup>		<u>0.7</u>				0.66	0.663	0.699				0.642
F	mg kg <sup>-1</sup>												
Ga	mg kg <sup>-1</sup>	<u>10</u>				<u>12</u>	7.57	8.804	8.11		11	8	<u>8.4</u>
Gd	mg kg <sup>-1</sup>		<u>1.8</u>				2.87	3.03	3.126			3.13	<u>3.06</u>
Ge	mg kg <sup>-1</sup>							0.648	1.07				
Hf	mg kg <sup>-1</sup>						8.06	8.502	8.289			8.31	<u>7.7</u>
Hg	mg kg <sup>-1</sup>												<u>0.084</u>
Ho	mg kg <sup>-1</sup>		<u>0.4</u>				0.624	0.585	0.634				0.602
I	mg kg <sup>-1</sup>												
In	mg kg <sup>-1</sup>												
La	mg kg <sup>-1</sup>	<u>22</u>	<u>26</u>				22.39	21.18	22.686		32	21.91	<u>23.1</u>
Li	mg kg <sup>-1</sup>		<u>21</u>				21.84	22.38				21.25	<u>23</u>
Lu	mg kg <sup>-1</sup>		<u>0.3</u>				0.279	0.283	0.288			0.266	<u>0.28</u>
Mo	mg kg <sup>-1</sup>						0.737	0.832	0.828				0.726
N	mg kg <sup>-1</sup>												
Nb	mg kg <sup>-1</sup>	<u>15</u>				<u>11</u>	14.94	17.06	14.784		15	14.55	<u>14.1</u>
Nd	mg kg <sup>-1</sup>		<u>18</u>				18.34	17.52	19.103		23	18.05	<u>19.4</u>
Ni	mg kg <sup>-1</sup>	<u>20</u>	<u>23</u>			<u>18</u>	18.44	18.96	21.56		53	20.91	<u>19.55</u>
Pb	mg kg <sup>-1</sup>	<u>27</u>	<u>30</u>			<u>28</u>	23.31	24.21	23.3		25		24.12
Pr	mg kg <sup>-1</sup>		<u>6</u>				5.08	4.652	5.408				4.96
Rb	mg kg <sup>-1</sup>	<u>55</u>	<u>51</u>				53.9	57.5	54.06		56	52.21	<u>53.8</u>
Re	mg kg <sup>-1</sup>												
S	mg kg <sup>-1</sup>									420			<u>1.25</u>
Sb	mg kg <sup>-1</sup>						1.299	1.521	2.812				
Sc	mg kg <sup>-1</sup>	<u>5</u>	<u>5</u>			<u>10</u>	5.47	5.934	5.79			5.78	<u>5.36</u>
Se	mg kg <sup>-1</sup>							0.551					
Sm	mg kg <sup>-1</sup>		<u>3.6</u>				3.28	3.184	3.335				3.25
Sn	mg kg <sup>-1</sup>						2.45	2.652	2.36				<u>2.4</u>
Sr	mg kg <sup>-1</sup>	<u>27</u>	<u>27</u>			<u>50</u>	26.8	25.7	27.6		35	28.2	<u>26.13</u>
Ta	mg kg <sup>-1</sup>						0.967	1.12	1.183				0.96
Tb	mg kg <sup>-1</sup>		<u>0.3</u>				0.463	0.527	0.494				0.499
Te	mg kg <sup>-1</sup>												
Th	mg kg <sup>-1</sup>		<u>5</u>				5.49	5.954	5.959		6		5.86
Tl	mg kg <sup>-1</sup>						0.316	0.316	0.353				0.31
Tm	mg kg <sup>-1</sup>		<u>0.2</u>				0.28	0.264	0.285				0.27
U	mg kg <sup>-1</sup>		<u>2</u>				2.085	2.15	2.159				2.01
V	mg kg <sup>-1</sup>	<u>60</u>	<u>55</u>			<u>74</u>	47.65	50.2	51.4		46	52.5	<u>46.77</u>
W	mg kg <sup>-1</sup>						1.09	1.634					<u>1.03</u>
Y	mg kg <sup>-1</sup>	<u>18</u>	<u>11.3</u>			<u>24</u>	17.1	18.88	18.83		19	22.47	<u>17.83</u>
Yb	mg kg <sup>-1</sup>		<u>1.4</u>				1.839	1.743	1.884				1.81
Zn	mg kg <sup>-1</sup>	<u>58</u>	<u>72</u>			<u>65</u>	62	61.3	77.3		61	65.97	<u>57.88</u>
Zr	mg kg <sup>-1</sup>	<u>318</u>	<u>275</u>			<u>290</u>	334	319	337.5	0.028	340		354.6

Bold entries are Data Quality 1 - Underlined entries are Data Quality 2

Table 1 - GeoPT47A Contributed data for Silty soil, NES-1. 20/11/2020

Lab Code	J72	J73	J74	J75	J76	J77	J79	J80	J81	J82	J83	J84	J85
SiO <sub>2</sub>	g 100g <sup>-1</sup>	<u>78.9</u>	79.4	<u>81.397</u>	79.61	<u>80.31</u>	78.02	80.36	<u>80.4</u>	79.93	79.3	79.1	79.06
TiO <sub>2</sub>	g 100g <sup>-1</sup>		<u>0.71</u>	<u>0.707</u>	0.71	<u>0.7</u>	0.754	0.698	0.7	<u>0.72</u>	<u>0.793</u>	0.67	0.711
Al <sub>2</sub> O <sub>3</sub>	g 100g <sup>-1</sup>		<u>6.3</u>	<u>5.818</u>	5.58	<u>5.7</u>	6.6	5.684	5.7	5.67	<u>6.31</u>	5.6	5.73
Fe <sub>2</sub> O <sub>3</sub> T	g 100g <sup>-1</sup>		<u>3.2</u>	<u>3.176</u>	3.1	<u>3.12</u>	3.28	3.15	<u>3.14</u>	3.08	<u>3.24</u>	3.07	<u>3.21</u>
Fe(II)O	g 100g <sup>-1</sup>						1.125	3.2		1.67		2.71	
MnO	g 100g <sup>-1</sup>			<u>0.094</u>	<u>0.099</u>	0.09		<u>0.114</u>	<u>0.093</u>	0.1	<u>0.086</u>	<u>0.087</u>	0.09
MgO	g 100g <sup>-1</sup>			<u>0.64</u>	<u>0.455</u>	0.48	<u>0.5</u>	<u>0.16</u>	<u>0.501</u>	<u>0.54</u>	<u>0.51</u>		0.48
CaO	g 100g <sup>-1</sup>			<u>0.34</u>	<u>0.279</u>	0.31	<u>0.31</u>	0.44	<u>0.311</u>	<u>0.35</u>	0.31	<u>0.646</u>	0.3
Na <sub>2</sub> O	g 100g <sup>-1</sup>			<u>0.32</u>	<u>0.291</u>	0.25	<u>0.28</u>	0.26	<u>0.286</u>	0.31	<u>0.35</u>		0.28
K <sub>2</sub> O	g 100g <sup>-1</sup>			<u>1.1</u>	<u>1.061</u>	1.05	<u>1.04</u>	1.14	<u>1.056</u>	1.03	<u>1.02</u>	<u>1.03</u>	1.05
P <sub>2</sub> O <sub>5</sub>	g 100g <sup>-1</sup>			<u>0.225</u>	<u>0.227</u>	0.22	<u>0.25</u>	<u>0.262</u>	<u>0.229</u>	0.23	<u>0.23</u>		0.23
H <sub>2</sub> O+	g 100g <sup>-1</sup>						<u>3.56</u>	5.6					
CO <sub>2</sub>	g 100g <sup>-1</sup>							<u>0.12</u>					
LOI	g 100g <sup>-1</sup>	<u>7.75</u>	<u>7.6</u>	<u>7.49</u>	<u>7.76</u>	<u>7.33</u>	<u>8.78</u>	<u>7.655</u>	7.5	<u>7.86</u>		<u>9.13</u>	<u>7.56</u>
Ag	mg kg <sup>-1</sup>						<u>0.124</u>	0.3	<u>0.34</u>			0.14	38.7
As	mg kg <sup>-1</sup>			<u>10</u>			<u>10.25</u>	<u>18.3</u>	<u>7.87</u>			<u>8.8</u>	10.3
Au	mg kg <sup>-1</sup>												14
B	mg kg <sup>-1</sup>							<u>16</u>			<u>34.3</u>		
Ba	mg kg <sup>-1</sup>		<u>158</u>	<u>150.060</u>	<u>165</u>	<u>147</u>	<u>200</u>	<u>163</u>	<u>153.5</u>	<u>166</u>		<u>160.5</u>	<u>176</u>
Be	mg kg <sup>-1</sup>		<u>0.83</u>	0.11		<u>0.68</u>	0.6	<u>0.67</u>	0.7			0.66	0.66
Bi	mg kg <sup>-1</sup>					<u>0.11</u>	<u>0.22</u>	0.2				0.13	0.09
Br	mg kg <sup>-1</sup>												
C(org)	mg kg <sup>-1</sup>						<u>10700</u>		<u>2.87</u>				1.93
C(tot)	mg kg <sup>-1</sup>							<u>29600</u>		<u>25650</u>			2.95
Cd	mg kg <sup>-1</sup>		<u>0.25</u>	<u>0.24</u>			<u>0.228</u>	<u>0.28</u>	<u>0.27</u>			<u>0.25</u>	<u>0.29</u>
Ce	mg kg <sup>-1</sup>		<u>42</u>	<u>36.86</u>		<u>47</u>	<u>58</u>	<u>45.9</u>	<u>42.9</u>			<u>42</u>	46.7
Cl	mg kg <sup>-1</sup>		<u>70</u>										
Co	mg kg <sup>-1</sup>		<u>9.09</u>	7.27			<u>8.27</u>	<u>10.6</u>	<u>8.37</u>	8.4		<u>8.4</u>	9.67
Cr	mg kg <sup>-1</sup>		<u>55</u>	<u>88.02</u>	<u>51</u>	<u>54.5</u>	<u>72</u>	62	<u>61.8</u>		<u>57.5</u>	<u>60</u>	65.1
Cs	mg kg <sup>-1</sup>			<u>2.29</u>			<u>2.55</u>	3.3	2.3	2.6	<u>2.03</u>		2.53
Cu	mg kg <sup>-1</sup>		<u>18.5</u>	<u>15.24</u>		<u>17.15</u>	<u>23.6</u>	<u>17.66</u>	18	<u>18</u>	<u>18.2</u>	19.8	36.6
Dy	mg kg <sup>-1</sup>		<u>1.95</u>	1.63		<u>3.11</u>	2.6	<u>3.94</u>	3		<u>2.04</u>	2.81	<u>2.9</u>
Er	mg kg <sup>-1</sup>		<u>1.16</u>	<u>0.99</u>		<u>1.95</u>	<u>1.53</u>	<u>2.12</u>	1.8		<u>1.74</u>	1.66	1.84
Eu	mg kg <sup>-1</sup>		<u>0.6</u>	0.54		<u>0.69</u>	0.71	<u>0.65</u>	0.7			0.72	0.67
F	mg kg <sup>-1</sup>		<u>500</u>										
Ga	mg kg <sup>-1</sup>		<u>8.62</u>	<u>6.94</u>	<u>10</u>	<u>7.26</u>	<u>11.05</u>	<u>7.31</u>	8.1			<u>7.97</u>	11.1
Gd	mg kg <sup>-1</sup>		<u>2.43</u>	2.47		<u>2.97</u>	2.9	<u>3.82</u>	2.9			2.44	3.13
Ge	mg kg <sup>-1</sup>			<u>1.76</u>			<u>1.87</u>	<u>1.31</u>				0.09	3.4
Hf	mg kg <sup>-1</sup>					<u>2.8</u>	<u>5.9</u>	<u>8.54</u>	8	<u>5.7</u>		<u>2.8</u>	4.37
Hg	mg kg <sup>-1</sup>					<u>0.079</u>							6.79
Ho	mg kg <sup>-1</sup>		<u>0.39</u>	0.32		<u>0.64</u>	<u>0.52</u>	<u>0.73</u>	0.6			0.41	0.54
I	mg kg <sup>-1</sup>												
In	mg kg <sup>-1</sup>											<u>0.027</u>	
La	mg kg <sup>-1</sup>		<u>21.4</u>	<u>19.34</u>	<u>20</u>	<u>23.7</u>	<u>26.4</u>	<u>31.1</u>	<u>22.2</u>			<u>23.3</u>	<u>24.4</u>
Li	mg kg <sup>-1</sup>		<u>21.2</u>	18.6		<u>20.6</u>	<u>20.8</u>	19	<u>20.2</u>			<u>20.1</u>	18.9
Lu	mg kg <sup>-1</sup>		<u>0.19</u>	0.15		<u>0.28</u>	0.23	<u>0.29</u>	0.3			<u>0.22</u>	0.22
Mo	mg kg <sup>-1</sup>		<u>0.73</u>	0.63		<u>0.65</u>	<u>2.2</u>	<u>0.81</u>	0.7			<u>0.8</u>	1.13
N	mg kg <sup>-1</sup>												
Nb	mg kg <sup>-1</sup>		<u>16</u>	<u>10.56</u>		<u>12.55</u>	<u>21.7</u>	<u>13.63</u>	<u>14.5</u>			<u>15.2</u>	<u>16.1</u>
Nd	mg kg <sup>-1</sup>		<u>17.8</u>	<u>15.91</u>		<u>20.2</u>	<u>21.3</u>	<u>20.8</u>	<u>18.3</u>			<u>19.8</u>	<u>19.6</u>
Ni	mg kg <sup>-1</sup>		<u>20</u>	16.3	<u>18</u>	<u>17.55</u>	<u>25.5</u>	<u>18.7</u>	<u>19.5</u>	<u>18.4</u>		<u>19.7</u>	21.9
Pb	mg kg <sup>-1</sup>		<u>25.3</u>	<u>20.55</u>		<u>25.1</u>	<u>29.5</u>	<u>21.2</u>	<u>25.1</u>		<u>17.4</u>	<u>25.4</u>	26.5
Pr	mg kg <sup>-1</sup>		<u>4.79</u>	4.91		<u>5.46</u>	5.9	<u>4.98</u>	4.9			<u>5.05</u>	5.47
Rb	mg kg <sup>-1</sup>		<u>55.3</u>	<u>47.72</u>		<u>52.7</u>	<u>62</u>	<u>51.5</u>	<u>53.3</u>		<u>53.2</u>	<u>52.5</u>	<u>52.5</u>
Re	mg kg <sup>-1</sup>												0.002
S	mg kg <sup>-1</sup>		<u>400</u>	<u>896.480</u>			<u>850</u>	<u>455</u>				0.04	
Sb	mg kg <sup>-1</sup>		<u>1.11</u>	1.05		<u>1.1</u>	1.7	<u>1.2</u>				<u>1.38</u>	1.84
Sc	mg kg <sup>-1</sup>		<u>4.85</u>	4.66	<u>5</u>	<u>5.12</u>	7.5		<u>5.2</u>			<u>5</u>	5.52
Se	mg kg <sup>-1</sup>			<u>0.46</u>		<u>0.493</u>	0.98					1	1.8
Sm	mg kg <sup>-1</sup>		<u>3.13</u>	2.82		<u>3.55</u>	3.7	<u>2.96</u>	3.3			<u>3.69</u>	3.47
Sn	mg kg <sup>-1</sup>		<u>1.75</u>			<u>1.74</u>	<u>3.2</u>	<u>5.09</u>	2.1			<u>1.7</u>	2.19
Sr	mg kg <sup>-1</sup>		<u>26.7</u>	<u>24.24</u>	<u>25</u>	<u>26.9</u>	<u>38.2</u>	<u>27.5</u>	<u>26.4</u>	<u>27</u>	<u>23.4</u>	<u>27.9</u>	<u>31.1</u>
Ta	mg kg <sup>-1</sup>					<u>0.77</u>	2.2	<u>0.9</u>	0.9			1	1.5
Tb	mg kg <sup>-1</sup>		<u>0.33</u>	0.31		<u>0.49</u>	0.39	<u>0.45</u>	0.5			0.44	0.43
Te	mg kg <sup>-1</sup>						<u>0.06</u>					0.05	
Th	mg kg <sup>-1</sup>				<u>2761.570</u>		<u>5.93</u>	7.1	<u>6.13</u>	5.8	<u>4.35</u>		<u>5.87</u>
Tl	mg kg <sup>-1</sup>		<u>0.34</u>	0.26		<u>0.277</u>	0.37			0.3		0.34	0.3
Tm	mg kg <sup>-1</sup>		<u>0.18</u>	0.14		<u>0.28</u>	0.23	<u>0.28</u>	0.3			<u>0.27</u>	0.21
U	mg kg <sup>-1</sup>		<u>2</u>	1.59		<u>1.92</u>	2.5	<u>2.49</u>	2.1			2	2.07
V	mg kg <sup>-1</sup>		<u>53.1</u>	41.79	<u>49</u>	<u>46.6</u>	64	42	<u>48.4</u>			<u>44</u>	<u>58.9</u>
W	mg kg <sup>-1</sup>					<u>0.867</u>	4.5	1.2				<u>0.8</u>	2.38
Y	mg kg <sup>-1</sup>		<u>19</u>	8.74		<u>18.4</u>	<u>14.9</u>	<u>16.1</u>	<u>18.2</u>			<u>17.5</u>	<u>16.2</u>
Yb	mg kg <sup>-1</sup>		<u>1.19</u>	1.01		<u>1.97</u>	<u>1.49</u>	2.2	1.8			1.88	1.65
Zn	mg kg <sup>-1</sup>		<u>66.9</u>	70.97	<u>59</u>	<u>62.1</u>	<u>57</u>	<u>65.2</u>	63	<u>64</u>	<u>64.5</u>	<u>67</u>	60.7
Zr	mg kg <sup>-1</sup>		<u>320</u>	<u>310.110</u>		<u>96.3</u>	<u>250</u>	<u>333</u>	<u>325.9</u>	<u>323</u>	<u>313.2</u>	<u>321</u>	174
													<u>287.6</u>

Bold entries are Data Quality 1 - Underlined entries are Data Quality 2

Table 1 - GeoPT47A Contributed data for Silty soil, NES-1. 20/11/2020

Lab Code	J87	J88	J89	J91	J92	J95	J96	J99	J100	J101	J102	J103	J105	
SiO <sub>2</sub>	g 100g <sup>-1</sup>	<b>64.69</b>	<u>80.12</u>	70.9	<u>79.92</u>		<b>79.52</b>	<u>80.33</u>	<b>81.17</b>		<u>80.3</u>	<b>66.53</b>	<u>80.4</u>	<b>79.63</b>
TiO <sub>2</sub>	g 100g <sup>-1</sup>	<b>0.672</b>	<u>0.696</u>	0.64	<u>0.74</u>		<b>0.672</b>	<u>0.707</u>	<b>0.76</b>		<u>0.7</u>	<b>0.79</b>	<u>0.753</u>	<b>0.68</b>
Al <sub>2</sub> O <sub>3</sub>	g 100g <sup>-1</sup>	<b>5.31</b>	<u>5.68</u>	7.55	<u>6.04</u>		<b>5.87</b>	<u>5.7</u>	<b>5.48</b>		<u>5.68</u>	<b>14.94</b>	<u>5.63</u>	<b>5.51</b>
Fe <sub>2</sub> O <sub>3</sub> T	g 100g <sup>-1</sup>	<b>2.911</b>	<u>3.16</u>	2.96	<u>3.54</u>		<b>3.43</b>	<u>3.15</u>	<b>3.06</b>		<u>3.29</u>	<b>6.25</b>	<u>3.2</u>	<b>3.12</b>
Fe(II)O	g 100g <sup>-1</sup>													
MnO	g 100g <sup>-1</sup>	<b>0.093</b>	<u>0.094</u>	0.141	<u>0.108</u>		<b>0.101</b>	<u>0.092</u>	<b>0.085</b>		<u>0.09</u>	<b>0.15</b>	<u>0.092</u>	<b>0.1</b>
MgO	g 100g <sup>-1</sup>	<b>0.533</b>	<u>0.5</u>		<u>0.59</u>		<b>0.486</b>	<u>0.513</u>	<b>0.49</b>		<u>0.5</u>	<b>2.27</b>	<u>0.532</u>	<b>0.37</b>
CaO	g 100g <sup>-1</sup>	<b>0.309</b>	<u>0.34</u>	<u>0.342</u>	<u>0.36</u>		<b>0.29</b>	<u>0.319</u>	<b>0.32</b>		<u>0.31</u>	<b>0.42</b>	<u>0.312</u>	<b>0.29</b>
Na <sub>2</sub> O	g 100g <sup>-1</sup>	<b>0.236</b>	<u>0.28</u>		<u>0.28</u>		<b>0.229</b>	<u>0.307</u>	<b>1.04</b>		<u>0.28</u>	<b>1.34</b>	<u>0.29</u>	<b>0.32</b>
K <sub>2</sub> O	g 100g <sup>-1</sup>	<b>1.046</b>	<u>1.04</u>	<u>1.1</u>	<u>1.1</u>		<b>1.062</b>	<u>1.07</u>	<b>0.23</b>		<u>1.05</u>	<b>2.77</b>	<u>1.06</u>	<b>0.96</b>
P <sub>2</sub> O <sub>5</sub>	g 100g <sup>-1</sup>	<b>0.229</b>	<u>0.227</u>		<u>0.25</u>		<b>0.244</b>	<u>0.224</u>	<b>0.27</b>		<u>0.23</u>	<b>0.17</b>	<u>0.228</u>	<b>0.17</b>
H <sub>2</sub> O+	g 100g <sup>-1</sup>													
CO <sub>2</sub>	g 100g <sup>-1</sup>											<u>6.63</u>		
LOI	g 100g <sup>-1</sup>		<u>7.69</u>		<u>7.81</u>		<b>8.266</b>	<u>7.44</u>	<b>8.02</b>		<u>7.58</u>	<b>4.25</b>	<u>7.77</u>	<b>8.88</b>
Ag	mg kg <sup>-1</sup>													
As	mg kg <sup>-1</sup>			<u>9.2</u>				<u>11.5</u>			<u>13.2</u>	<b>24</b>		
Au	mg kg <sup>-1</sup>													
B	mg kg <sup>-1</sup>													
Ba	mg kg <sup>-1</sup>		<u>150</u>	<u>156</u>	<u>155</u>		<b>163.8</b>	<u>161.150</u>		<b>192.6</b>	<u>160.4</u>	<b>422</b>		
Be	mg kg <sup>-1</sup>						<b>0.741</b>	<u>1.03</u>		<b>0.961</b>	<u>0.95</u>			
Bi	mg kg <sup>-1</sup>									<b>0.143</b>	<u>0.13</u>			
Br	mg kg <sup>-1</sup>			<u>15</u>				<u>15.5</u>						
C(org)	mg kg <sup>-1</sup>			<u>26852</u>								<u>11400</u>		
C(tot)	mg kg <sup>-1</sup>	<b>2.967</b>	<u>28186</u>									<u>29500</u>		
Cd	mg kg <sup>-1</sup>											<u>0.3</u>		
Ce	mg kg <sup>-1</sup>			<u>42.4</u>			<b>43</b>	<u>43.21</u>		<b>51.7</b>	<u>44.1</u>	<b>80.58</b>		
Cl	mg kg <sup>-1</sup>		<u>100</u>					<u>113</u>						
Co	mg kg <sup>-1</sup>				<u>7.7</u>		<b>8.61</b>	<u>8.17</u>		<b>9.511</b>	<u>8.48</u>			
Cr	mg kg <sup>-1</sup>		<u>76</u>	<u>68.6</u>	<u>66</u>		<b>45.18</b>	<u>57.8</u>		<b>71.77</b>	<u>48.1</u>	<b>131</b>		
Cs	mg kg <sup>-1</sup>						<b>2.874</b>	<u>2.86</u>		<b>2.846</b>		<b>6.3</b>		
Cu	mg kg <sup>-1</sup>		<u>19</u>	<u>23.2</u>	<u>21</u>		<b>17.78</b>	<u>17.3</u>		<b>19.1</b>	<u>19.9</u>	<b>40</b>		
Dy	mg kg <sup>-1</sup>						<b>2.1</b>	<u>3.02</u>		<b>2.99</b>	<u>3.03</u>	<b>5.63</b>		
Er	mg kg <sup>-1</sup>						<b>1.21</b>	<u>1.94</u>		<b>1.818</b>	<u>1.93</u>	<b>3.08</b>		
Eu	mg kg <sup>-1</sup>						<b>0.63</b>	<u>0.69</u>		<b>0.783</b>	<u>0.69</u>	<b>1.6</b>		
F	mg kg <sup>-1</sup>				<u>284</u>			<u>465</u>				<u>324.3</u>		
Ga	mg kg <sup>-1</sup>		<u>10</u>		<u>9.4</u>		<b>7.97</b>	<u>8.8</u>		<b>9.912</b>	<u>8.81</u>			
Gd	mg kg <sup>-1</sup>						<b>2.53</b>	<u>2.97</u>		<b>3.292</b>	<u>3.07</u>	<b>6.12</b>		
Ge	mg kg <sup>-1</sup>							<u>1.48</u>				<u>2.86</u>		
Hf	mg kg <sup>-1</sup>		<u>8.5</u>				<b>3</b>	<u>8.35</u>		<b>5.177</b>	<u>6.87</u>	<b>6.02</b>		
Hg	mg kg <sup>-1</sup>									<b>0.071</b>				
Ho	mg kg <sup>-1</sup>						<b>2.1</b>	<u>0.63</u>		<b>0.624</b>	<u>0.64</u>	<b>1.11</b>		
I	mg kg <sup>-1</sup>													
In	mg kg <sup>-1</sup>											<u>0.03</u>		
La	mg kg <sup>-1</sup>		<u>20.2</u>				<b>22.45</b>	<u>23.82</u>		<b>26.64</b>	<u>22.5</u>	<b>34.5</b>		
Li	mg kg <sup>-1</sup>							<u>23.12</u>			<u>24.23</u>	<u>18.8</u>		
Lu	mg kg <sup>-1</sup>							<u>0.194</u>	<u>0.31</u>		<u>0.269</u>	<u>0.28</u>	<b>0.43</b>	
Mo	mg kg <sup>-1</sup>							<u>0.678</u>			<u>0.95</u>	<u>0.7</u>	<b>1.04</b>	
N	mg kg <sup>-1</sup>	<b>0.329</b>												
Nb	mg kg <sup>-1</sup>	<u>11</u>	<u>18.9</u>	<u>17</u>			<b>13.24</b>	<u>14.28</u>		<b>15.65</b>	<u>9.89</u>	<b>14.88</b>		
Nd	mg kg <sup>-1</sup>			<u>19</u>				<u>18.2</u>	<u>18.38</u>		<b>21.86</b>	<u>18.8</u>	<b>34.35</b>	
Ni	mg kg <sup>-1</sup>		<u>21</u>		<u>20</u>			<b>19.05</b>	<u>19.4</u>		<b>21.03</b>	<u>21.7</u>	<b>80</b>	
Pb	mg kg <sup>-1</sup>		<u>28.3</u>	<u>31</u>			<b>26.22</b>	<u>26.3</u>		<b>29.03</b>	<u>24.4</u>	<b>37.4</b>		
Pr	mg kg <sup>-1</sup>						<b>5.08</b>	<u>5.04</u>		<b>5.709</b>	<u>5</u>	<b>9.07</b>		
Rb	mg kg <sup>-1</sup>		<u>48</u>	<u>56.3</u>			<b>57.02</b>	<u>54.99</u>		<b>71.27</b>	<u>52.8</u>	<b>99</b>		
Re	mg kg <sup>-1</sup>													
S	mg kg <sup>-1</sup>	<b>0.049</b>						<u>573</u>			<u>459</u>			
Sb	mg kg <sup>-1</sup>									<b>1.264</b>	<u>1.43</u>			
Sc	mg kg <sup>-1</sup>			<u>5.4</u>			<b>5.4</b>			<b>6.28</b>	<u>5.23</u>	<b>17.69</b>		
Se	mg kg <sup>-1</sup>											<u>1.15</u>		
Sm	mg kg <sup>-1</sup>						<b>3.21</b>	<u>3.36</u>		<b>3.788</b>	<u>3.46</u>	<b>6.83</b>		
Sn	mg kg <sup>-1</sup>									<b>1.508</b>	<u>2.02</u>			
Sr	mg kg <sup>-1</sup>	<u>30</u>	<u>27.2</u>	<u>30</u>			<b>27.5</b>	<u>27.6</u>		<b>33.58</b>	<u>27</u>	<b>68</b>		
Ta	mg kg <sup>-1</sup>						<b>0.769</b>	<u>1.11</u>		<b>1.06</b>	<u>0.65</u>	<b>1.01</b>		
Tb	mg kg <sup>-1</sup>						<b>0.36</b>	<u>0.5</u>		<b>0.512</b>	<u>0.49</u>	<b>0.99</b>		
Te	mg kg <sup>-1</sup>													
Th	mg kg <sup>-1</sup>		<u>5.1</u>				<b>6.054</b>	<u>6.08</u>		<b>6.538</b>	<u>5.35</u>	<b>9.71</b>		
Tl	mg kg <sup>-1</sup>											<u>0.31</u>		
Tm	mg kg <sup>-1</sup>							<u>0.29</u>		<b>0.262</b>	<u>0.29</u>	<b>0.45</b>		
U	mg kg <sup>-1</sup>		<u>1.43</u>				<b>1.93</b>	<u>2.23</u>		<b>2.108</b>	<u>2.29</u>	<b>3.2</b>		
V	mg kg <sup>-1</sup>		<u>49</u>		<u>50</u>		<b>49.28</b>	<u>51.76</u>		<b>52.17</b>	<u>47.1</u>	<b>121</b>		
W	mg kg <sup>-1</sup>						<b>0.64</b>	<u>5.06</u>			<u>0.67</u>			
Y	mg kg <sup>-1</sup>		<u>19</u>	<u>12.7</u>	<u>20</u>		<b>12.49</b>	<u>18.24</u>		<b>18.38</b>	<u>16.9</u>	<b>33.5</b>		
Yb	mg kg <sup>-1</sup>						<b>1.29</b>	<u>1.92</u>		<b>1.781</b>	<u>1.83</u>	<b>2.98</b>		
Zn	mg kg <sup>-1</sup>		<u>68</u>	<u>58</u>	<u>74</u>		<b>64.22</b>	<u>65.1</u>		<b>70.33</b>	<u>65</u>	<b>110</b>		
Zr	mg kg <sup>-1</sup>		<u>330</u>	<u>295.5</u>	<u>356</u>		<b>109.9</b>	<u>339.6</u>		<b>227.4</b>	<u>317.2</u>	<b>234.5</b>		

Bold entries are Data Quality 1 - Underlined entries are Data Quality 2

Table 1 - GeoPT47A Contributed data for Silty soil, NES-1. 20/11/2020

Lab Code	J106	J108	J109	J112	J116	J117	J118	J120	J121	J122	J123	J124	J126
SiO <sub>2</sub>	g 100g <sup>-1</sup>	<u>80.15</u>	80.8	<u>80.78</u>	80.4	<u>79.61</u>	79.98	<u>80.43</u>	<u>80.46</u>	<u>80.03</u>	<u>78.99</u>	<u>80.2</u>	<u>79.017</u>
TiO <sub>2</sub>	g 100g <sup>-1</sup>	<u>0.714</u>	<u>0.69</u>	0.7	<u>0.71</u>	<u>0.7</u>	<u>0.736</u>	<u>0.7</u>	<u>0.74</u>	<u>0.7</u>	<u>0.709</u>	<u>0.68</u>	<u>0.682</u>
Al <sub>2</sub> O <sub>3</sub>	g 100g <sup>-1</sup>	<u>5.625</u>	<u>5.83</u>	5.67	<u>5.76</u>	<u>5.65</u>	<u>5.66</u>	<u>5.68</u>	<u>5.64</u>	<u>5.84</u>	<u>5.79</u>	<u>5.72</u>	<u>5.668</u>
Fe <sub>2</sub> O <sub>3</sub> T	g 100g <sup>-1</sup>	<u>3.093</u>	<u>3.09</u>	<u>3.05</u>	<u>3.18</u>	<u>3.07</u>	<u>3.123</u>	<u>3.1</u>	<u>3.18</u>	<u>3.16</u>	<u>3.05</u>	<u>3.09</u>	<u>3.19</u>
Fe(II)O	g 100g <sup>-1</sup>												
MnO	g 100g <sup>-1</sup>	<u>0.086</u>			<u>0.090</u>	<u>0.08</u>	<u>0.091</u>	<u>0.09</u>	0.1	<u>0.091</u>	<u>0.091</u>	<u>0.09</u>	<u>0.096</u>
MgO	g 100g <sup>-1</sup>	<u>0.513</u>	<u>0.49</u>	<u>0.49</u>	<u>0.51</u>	<u>0.49</u>	<u>0.488</u>	<u>0.5</u>	<u>0.49</u>	<u>0.502</u>	<u>0.46</u>	<u>0.53</u>	<u>0.523</u>
CaO	g 100g <sup>-1</sup>	<u>0.313</u>	<u>0.3</u>	<u>0.32</u>	<u>0.33</u>	<u>0.32</u>	<u>0.311</u>	<u>0.31</u>	<u>0.38</u>	<u>0.347</u>	<u>0.31</u>	<u>0.49</u>	<u>0.269</u>
Na <sub>2</sub> O	g 100g <sup>-1</sup>	<u>0.257</u>	<u>0.3</u>	<u>0.3</u>	<u>0.28</u>	<u>0.25</u>	<u>0.271</u>	<u>0.28</u>	<u>0.12</u>	<u>0.277</u>	<u>0.35</u>	<u>0.38</u>	<u>0.284</u>
K <sub>2</sub> O	g 100g <sup>-1</sup>	<u>1.042</u>	<u>1.02</u>	<u>1.05</u>	<u>1.04</u>	<u>1.05</u>	<u>0.944</u>	<u>1.05</u>	1	<u>1.089</u>	<u>1.07</u>	<u>1.02</u>	<u>1.036</u>
P <sub>2</sub> O <sub>5</sub>	g 100g <sup>-1</sup>		<u>0.22</u>	<u>0.26</u>	<u>0.23</u>	<u>0.23</u>	<u>0.23</u>	<u>0.23</u>	<u>0.22</u>	<u>0.222</u>	<u>0.23</u>	<u>0.23</u>	<u>0.224</u>
H <sub>2</sub> O+	g 100g <sup>-1</sup>			<u>1.59</u>									
CO <sub>2</sub>	g 100g <sup>-1</sup>												
LOI	g 100g <sup>-1</sup>	<u>7.911</u>	<u>7.36</u>	7.71		<u>8.22</u>	<u>7.665</u>	<u>7.35</u>	8.03	<u>7.35</u>	<u>7.9</u>	<u>8.01</u>	
Ag	mg kg <sup>-1</sup>					<u>0.123</u>					<u>0.28</u>		
As	mg kg <sup>-1</sup>					<u>8.36</u>			10		<u>12</u>	<u>9.7</u>	
Au	mg kg <sup>-1</sup>												
B	mg kg <sup>-1</sup>												
Ba	mg kg <sup>-1</sup>					<u>164</u>		<u>152</u>	<u>156</u>	<u>202</u>	<u>154</u>	<u>147</u>	<u>179.5</u>
Be	mg kg <sup>-1</sup>					<u>1.02</u>		<u>0.8</u>			<u>0.73</u>	<u>0.7</u>	
Bi	mg kg <sup>-1</sup>					<u>0.13</u>		<u>0.12</u>					
Br	mg kg <sup>-1</sup>										<u>16</u>		
C(org)	mg kg <sup>-1</sup>												
C(tot)	mg kg <sup>-1</sup>	<u>29900</u>		<u>26480</u>				<u>24400</u>					<u>28500</u>
Cd	mg kg <sup>-1</sup>					<u>0.3</u>		<u>0.24</u>			<u>0.25</u>		
Ce	mg kg <sup>-1</sup>					<u>44.2</u>		<u>41.7</u>	<u>44.9</u>		<u>37.8</u>	<u>41.8</u>	<u>44</u>
Cl	mg kg <sup>-1</sup>												
Co	mg kg <sup>-1</sup>					<u>8.42</u>		<u>8.3</u>	12		<u>9</u>	<u>9.5</u>	
Cr	mg kg <sup>-1</sup>					<u>71.4</u>		<u>69</u>	<u>70</u>	<u>60</u>	<u>62</u>	<u>62.2</u>	<u>63</u>
Cs	mg kg <sup>-1</sup>					<u>2.91</u>		<u>2.62</u>	<u>2.6</u>		<u>2.74</u>	<u>2.5</u>	
Cu	mg kg <sup>-1</sup>					<u>17.1</u>		<u>18</u>	<u>23</u>	<u>23</u>	<u>20</u>	<u>18.6</u>	<u>25</u>
Dy	mg kg <sup>-1</sup>					<u>3.21</u>		<u>2.83</u>	<u>2.9</u>		<u>1.67</u>	<u>2.8</u>	
Er	mg kg <sup>-1</sup>					<u>1.86</u>		<u>1.8</u>	<u>1.8</u>		<u>1</u>	<u>1.7</u>	
Eu	mg kg <sup>-1</sup>					<u>0.7</u>		<u>0.64</u>	<u>0.8</u>		<u>0.59</u>	<u>0.7</u>	
F	mg kg <sup>-1</sup>												
Ga	mg kg <sup>-1</sup>					<u>8.21</u>		<u>8.14</u>	<u>7.5</u>		<u>5</u>	<u>7.7</u>	
Gd	mg kg <sup>-1</sup>					<u>3.1</u>		<u>2.79</u>	<u>2.93</u>		<u>2.01</u>	<u>3.1</u>	
Ge	mg kg <sup>-1</sup>					<u>1.27</u>		<u>1.1</u>					
Hf	mg kg <sup>-1</sup>					<u>8.96</u>		<u>8.23</u>	<u>7.8</u>		<u>5</u>	<u>8.1</u>	
Hg	mg kg <sup>-1</sup>												
Ho	mg kg <sup>-1</sup>					<u>0.63</u>		<u>0.6</u>	<u>0.7</u>		<u>0.34</u>	<u>0.6</u>	
I	mg kg <sup>-1</sup>												
In	mg kg <sup>-1</sup>												
La	mg kg <sup>-1</sup>					<u>23.1</u>		<u>22</u>	<u>22.9</u>	33		<u>19.5</u>	<u>22.5</u>
Li	mg kg <sup>-1</sup>					<u>21.5</u>			<u>19.5</u>			<u>20.5</u>	
Lu	mg kg <sup>-1</sup>					<u>0.3</u>		<u>0.27</u>	<u>0.3</u>		<u>0.15</u>	<u>0.3</u>	
Mo	mg kg <sup>-1</sup>					<u>0.77</u>		<u>0.7</u>	<u>46</u>		<u>0.72</u>	<u>0.8</u>	
N	mg kg <sup>-1</sup>												
Nb	mg kg <sup>-1</sup>					<u>14.4</u>		<u>13</u>	<u>14.2</u>	19		<u>15</u>	<u>13.8</u>
Nd	mg kg <sup>-1</sup>					<u>18.4</u>		<u>18</u>	<u>18.9</u>		<u>16.2</u>	<u>17.9</u>	
Ni	mg kg <sup>-1</sup>					<u>20.5</u>		<u>19</u>	27		<u>17</u>	<u>18.3</u>	<u>24</u>
Pb	mg kg <sup>-1</sup>					<u>25.9</u>		<u>25</u>	<u>35</u>	<u>32</u>	<u>25</u>	<u>26</u>	
Pr	mg kg <sup>-1</sup>					<u>5.11</u>		<u>4.96</u>	<u>5.2</u>		<u>4.5</u>	<u>5.1</u>	
Rb	mg kg <sup>-1</sup>					<u>54.4</u>		<u>51.5</u>	<u>52.3</u>	77	<u>54</u>	<u>55</u>	<u>51.9</u>
Re	mg kg <sup>-1</sup>												
S	mg kg <sup>-1</sup>	<u>411</u>				<u>361</u>		<u>200</u>	<u>481</u>				
Sb	mg kg <sup>-1</sup>					<u>1.33</u>		<u>1.1</u>			<u>1.03</u>		
Sc	mg kg <sup>-1</sup>					<u>5.93</u>		<u>5</u>			<u>5.4</u>	<u>5.2</u>	
Se	mg kg <sup>-1</sup>					<u>1.32</u>							
Sm	mg kg <sup>-1</sup>					<u>3.5</u>		<u>3.3</u>	<u>3.3</u>		<u>2.9</u>	<u>3.2</u>	
Sn	mg kg <sup>-1</sup>					<u>2.12</u>		<u>1.6</u>			<u>1.6</u>	<u>1.9</u>	
Sr	mg kg <sup>-1</sup>					<u>27.6</u>		<u>26.6</u>	<u>28.8</u>	<u>44</u>	<u>38</u>	<u>26.8</u>	<u>31.1</u>
Ta	mg kg <sup>-1</sup>					<u>1.1</u>		<u>0.97</u>	<u>1</u>			<u>1.3</u>	
Tb	mg kg <sup>-1</sup>					<u>0.49</u>		<u>0.45</u>	<u>0.5</u>			<u>0.29</u>	<u>0.5</u>
Te	mg kg <sup>-1</sup>												
Th	mg kg <sup>-1</sup>					<u>6.15</u>		<u>5.74</u>	<u>5.7</u>	17		<u>5.18</u>	<u>5.9</u>
Tl	mg kg <sup>-1</sup>					<u>0.33</u>		<u>0.3</u>				<u>0.29</u>	
Tm	mg kg <sup>-1</sup>					<u>0.29</u>		<u>0.28</u>	<u>0.3</u>			<u>0.15</u>	<u>0.3</u>
U	mg kg <sup>-1</sup>					<u>2.21</u>		<u>2.19</u>	<u>2.3</u>	<u>10</u>		<u>1.78</u>	<u>2.1</u>
V	mg kg <sup>-1</sup>					<u>52.9</u>		<u>48</u>	<u>60</u>	<u>56</u>	<u>53</u>	<u>48.9</u>	<u>51</u>
W	mg kg <sup>-1</sup>					<u>1.11</u>						<u>1.2</u>	
Y	mg kg <sup>-1</sup>					<u>19</u>		<u>16.8</u>	<u>17.6</u>	24		<u>19</u>	<u>18.5</u>
Yb	mg kg <sup>-1</sup>					<u>1.94</u>		<u>1.72</u>	<u>1.87</u>			<u>0.99</u>	<u>1.8</u>
Zn	mg kg <sup>-1</sup>					<u>66.5</u>		<u>65</u>	87	<u>60</u>	<u>62</u>	<u>52.5</u>	<u>65</u>
Zr	mg kg <sup>-1</sup>		<u>330</u>			<u>316</u>		<u>327</u>	<u>320</u>	<u>392</u>	<u>328</u>	<u>270</u>	<u>350.7</u>

Bold entries are Data Quality 1 - Underlined entries are Data Quality 2

Table 1 - GeoPT47A Contributed data for Silty soil, NES-1. 20/11/2020

Lab Code	J128	-	-	-	-	-	-	-	-	-	-	-	-
SiO <sub>2</sub>	g 100g <sup>-1</sup>	<b>80.64</b>											
TiO <sub>2</sub>	g 100g <sup>-1</sup>	<b>0.67</b>											
Al <sub>2</sub> O <sub>3</sub>	g 100g <sup>-1</sup>	<b>5.68</b>											
Fe <sub>2</sub> O <sub>3T</sub>	g 100g <sup>-1</sup>	<b>3.17</b>											
Fe(II)O	g 100g <sup>-1</sup>												
MnO	g 100g <sup>-1</sup>	<b>0.09</b>											
MgO	g 100g <sup>-1</sup>	<b>0.53</b>											
CaO	g 100g <sup>-1</sup>	<b>0.3</b>											
Na <sub>2</sub> O	g 100g <sup>-1</sup>	<b>0.3</b>											
K <sub>2</sub> O	g 100g <sup>-1</sup>	<b>1.05</b>											
P <sub>2</sub> O <sub>5</sub>	g 100g <sup>-1</sup>	<b>0.23</b>											
H <sub>2</sub> O+	g 100g <sup>-1</sup>												
CO <sub>2</sub>	g 100g <sup>-1</sup>												
LOI	g 100g <sup>-1</sup>	<b>7.24</b>											
Ag	mg kg <sup>-1</sup>												
As	mg kg <sup>-1</sup>	<b>11</b>											
Au	mg kg <sup>-1</sup>												
B	mg kg <sup>-1</sup>												
Ba	mg kg <sup>-1</sup>	<b>204</b>											
Be	mg kg <sup>-1</sup>												
Bi	mg kg <sup>-1</sup>												
Br	mg kg <sup>-1</sup>	<b>19</b>											
C(org)	mg kg <sup>-1</sup>												
C(tot)	mg kg <sup>-1</sup>												
Cd	mg kg <sup>-1</sup>												
Ce	mg kg <sup>-1</sup>	<b>48</b>											
Cl	mg kg <sup>-1</sup>												
Co	mg kg <sup>-1</sup>	<b>3</b>											
Cr	mg kg <sup>-1</sup>	<b>62</b>											
Cs	mg kg <sup>-1</sup>	<b>10</b>											
Cu	mg kg <sup>-1</sup>	<b>13</b>											
Dy	mg kg <sup>-1</sup>												
Er	mg kg <sup>-1</sup>												
Eu	mg kg <sup>-1</sup>												
F	mg kg <sup>-1</sup>	<b>665</b>											
Ga	mg kg <sup>-1</sup>	<b>10</b>											
Gd	mg kg <sup>-1</sup>	<b>3</b>											
Ge	mg kg <sup>-1</sup>	<b>2</b>											
Hf	mg kg <sup>-1</sup>	<b>12</b>											
Hg	mg kg <sup>-1</sup>												
Ho	mg kg <sup>-1</sup>												
I	mg kg <sup>-1</sup>												
In	mg kg <sup>-1</sup>												
La	mg kg <sup>-1</sup>	<b>30</b>											
Li	mg kg <sup>-1</sup>												
Lu	mg kg <sup>-1</sup>												
Mo	mg kg <sup>-1</sup>												
N	mg kg <sup>-1</sup>												
Nb	mg kg <sup>-1</sup>	<b>18</b>											
Nd	mg kg <sup>-1</sup>	<b>20</b>											
Ni	mg kg <sup>-1</sup>	<b>24</b>											
Pb	mg kg <sup>-1</sup>	<b>27</b>											
Pr	mg kg <sup>-1</sup>												
Rb	mg kg <sup>-1</sup>	<b>60</b>											
Re	mg kg <sup>-1</sup>												
S	mg kg <sup>-1</sup>	<b>365</b>											
Sb	mg kg <sup>-1</sup>												
Sc	mg kg <sup>-1</sup>	<b>8</b>											
Se	mg kg <sup>-1</sup>												
Sm	mg kg <sup>-1</sup>												
Sn	mg kg <sup>-1</sup>												
Sr	mg kg <sup>-1</sup>	<b>26</b>											
Ta	mg kg <sup>-1</sup>												
Tb	mg kg <sup>-1</sup>												
Te	mg kg <sup>-1</sup>												
Th	mg kg <sup>-1</sup>	<b>4</b>											
Tl	mg kg <sup>-1</sup>												
Tm	mg kg <sup>-1</sup>												
U	mg kg <sup>-1</sup>	<b>2</b>											
V	mg kg <sup>-1</sup>	<b>60</b>											
W	mg kg <sup>-1</sup>												
Y	mg kg <sup>-1</sup>	<b>21</b>											
Yb	mg kg <sup>-1</sup>												
Zn	mg kg <sup>-1</sup>	<b>68</b>											
Zr	mg kg <sup>-1</sup>	<b>296</b>											

**Bold entries** are Data Quality 1 - Underlined entries are Data Quality 2

Table 2 - GeoPT47A Consensus values and statistical summary for Silty soil, NES-1.

	Consensus Value	Uncertainty of consensus value	Horwitz Target Value	Uncertainty/Target	Number of reported results	Robust Mean of results	Robust SD of results	Median of results	Status of consensus value	Type of consensus value
	$X_a$	$sdm$	$H_a$	$edn/H_a$	$n$					
	$g\ 100g^{-1}$	$g\ 100g^{-1}$	$g\ 100g^{-1}$			$g\ 100g^{-1}$	$g\ 100g^{-1}$	$g\ 100g^{-1}$		
SiO <sub>2</sub>	80.15	0.0599	0.8287	0.07228	84	79.73	0.8885	79.93	Assigned	Mode
TiO <sub>2</sub>	0.7	0.003586	0.01477	0.2427	87	0.6983	0.02773	0.7	Assigned	Median
Al <sub>2</sub> O <sub>3</sub>	5.67	0.01594	0.08734	0.1825	87	5.671	0.1361	5.67	Assigned	Median
Fe <sub>2</sub> O <sub>3</sub> T	3.121	0.0161	0.05259	0.3061	87	3.143	0.09556	3.127	Assigned	Mode
MnO	0.09105	0.0004156	0.002612	0.1591	84	0.09257	0.005792	0.09105	Assigned	Median
MgO	0.5013	0.003268	0.01112	0.2937	85	0.5013	0.03013	0.5	Assigned	Robust Mean
CaO	0.32	0.002391	0.007597	0.3147	87	0.3261	0.03035	0.32	Provisional	Median
K <sub>2</sub> O	1.045	0.003158	0.02076	0.1521	87	1.045	0.02945	1.05	Assigned	Robust Mean
P <sub>2</sub> O <sub>5</sub>	0.23	0.0007845	0.005739	0.1367	81	0.2283	0.007187	0.23	Assigned	Median
LOI	7.641	0.0489	0.1125	0.4346	74	7.811	0.441	7.7	Provisional	Mode
	$mg\ kg^{-1}$	$mg\ kg^{-1}$	$mg\ kg^{-1}$			$mg\ kg^{-1}$	$mg\ kg^{-1}$	$mg\ kg^{-1}$		
As	10.04	0.316	0.5675	0.5568	35	10.67	2.291	10.2	Provisional	Mode
Ba	160.5	1.2	5.978	0.2007	69	164.6	13.94	161.7	Assigned	Mode
Be	0.71	0.0161	0.05979	0.2693	30	0.7771	0.1343	0.73	Assigned	Mode
Bi	0.13	0.00665	0.01413	0.4705	20	0.1449	0.0363	0.1315	Provisional	Mode
Cd	0.2689	0.009207	0.02621	0.3512	25	0.2689	0.04603	0.27	Provisional	Robust Mean
Ce	43	0.204	1.953	0.1045	55	43.94	3.302	43.45	Assigned	Mode
Co	8.385	0.045	0.487	0.09241	45	8.686	0.8042	8.5	Assigned	Mode
Cr	62.2	1.198	2.672	0.4485	65	63.06	8.375	62.2	Provisional	Median
Cs	2.64	0.0591	0.1825	0.3239	41	2.783	0.3652	2.723	Assigned	Mode
Cu	18	0.464	0.9319	0.4979	63	18.81	3.119	18.42	Assigned	Mode
Dy	2.953	0.0692	0.2007	0.3448	41	2.785	0.4762	2.9	Assigned	Mode
Er	1.818	0.0278	0.1329	0.2092	40	1.745	0.229	1.798	Assigned	Mode
Eu	0.68	0.0149	0.05764	0.2585	40	0.6753	0.04458	0.6775	Assigned	Mode
Ga	8.066	0.144	0.4712	0.3056	51	8.58	1.367	8.21	Provisional	Mode
Gd	2.93	0.093	0.1993	0.4665	41	2.907	0.2578	2.9	Assigned	Mode
Hf	8.1	0.136	0.4729	0.2876	44	6.779	2.427	7.75	Provisional	Mode
Ho	0.62	0.00602	0.05329	0.113	40	0.5851	0.1004	0.6065	Assigned	Mode
La	22.79	0.3574	1.139	0.3139	58	23.25	2.89	22.79	Assigned	Median
Li	21.23	0.3647	1.072	0.3402	30	21.36	1.751	21.23	Assigned	Median
Lu	0.29	0.003	0.02795	0.1074	40	0.2665	0.04314	0.28	Assigned	Mode
Mo	0.715	0.0225	0.06015	0.3741	34	0.808	0.189	0.7415	Assigned	Mode
Nb	14.44	0.2475	0.7727	0.3203	56	14.44	1.852	14.5	Assigned	Robust Mean
Nd	18.57	0.2023	0.9569	0.2114	54	18.8	1.446	18.57	Assigned	Median
Ni	19.05	0.45	0.9779	0.4602	60	19.83	2.505	19.52	Assigned	Mode
Pb	25.1	0.379	1.236	0.3067	56	25.78	2.986	25.28	Assigned	Mode
Pr	5.04	0.04063	0.316	0.1286	41	5.075	0.29	5.04	Assigned	Median
Rb	54	0.472	2.37	0.1992	62	54.58	4.022	54	Assigned	Median
Sb	1.159	0.08725	0.09063	0.9627	27	1.255	0.2298	1.25	Provisional	Mode
Sc	5.3	0.106	0.3298	0.3214	48	5.563	0.7206	5.4	Assigned	Mode
Sm	3.3	0.04482	0.2205	0.2032	44	3.333	0.2609	3.3	Assigned	Median
Sn	1.98	0.14	0.1429	0.9797	32	2.111	0.4712	2.06	Provisional	Mode
Sr	27	0.3	1.315	0.2281	68	28.15	2.833	27.52	Assigned	Mode
Ta	0.939	0.03	0.07582	0.3957	36	1.002	0.1733	0.975	Assigned	Mode
Tb	0.4665	0.008814	0.04185	0.2106	40	0.4543	0.0594	0.4665	Assigned	Median
Th	5.82	0.08066	0.3571	0.2259	51	5.852	0.6462	5.82	Assigned	Median
Tl	0.316	0.005946	0.03006	0.1978	25	0.3181	0.03144	0.316	Assigned	Median
Tm	0.28	0.005356	0.02712	0.1975	39	0.2655	0.03398	0.28	Assigned	Median
U	2.09	0.0238	0.1496	0.1591	50	2.174	0.2553	2.126	Assigned	Mode
V	51	0.7897	2.257	0.3499	64	51.72	6.524	51	Provisional	Median
W	1.06	0.0435	0.08404	0.5176	25	1.355	0.7025	1.09	Provisional	Mode
Y	17.8	0.2575	0.9231	0.279	63	17.68	2.051	17.8	Assigned	Median
Yb	1.82	0.0225	0.133	0.1691	42	1.729	0.2661	1.8	Assigned	Mode
Zn	64.11	0.633	2.741	0.2309	70	64.3	4.883	64.11	Assigned	Median
Zr	322	2.23	10.8	0.2065	70	309.4	36.25	318.5	Assigned	Mode

Table 3 - GeoPT47A Z-scores for Silty soil, NES-1. 20/11/2020

Lab Code	J1	J2	J3	J4	J5	J6	J9	J11	J12	J14	J15	J16	J18
SiO <sub>2</sub>	-20.79	<u>0.00</u>	-1.75	-0.63	*	*	-1.41	0.01	-1.70	0.35	0.07	-0.03	1.66
TiO <sub>2</sub>	27.76	<u>-0.14</u>	-2.03	<u>0.34</u>	<u>-16.92</u>	*	-0.41	-2.71	-2.78	1.35	<u>-0.68</u>	<u>-1.12</u>	-3.05
Al <sub>2</sub> O <sub>3</sub>	90.34	<u>0.50</u>	-1.49	<u>-0.17</u>	-2.86	*	-0.76	-2.18	-0.69	0.46	<u>-0.63</u>	<u>0.14</u>	-6.64
Fe <sub>2</sub> O <sub>3T</sub>	111.59	<u>-0.17</u>	-3.44	<u>0.97</u>	-0.78	*	-1.05	-1.35	-0.02	-0.40	<u>0.28</u>	<u>-0.19</u>	-4.57
MnO	34.06	<u>0.18</u>	-0.02	<u>-0.39</u>	1.51	*	-0.02	-0.40	-0.59	-0.02	<u>-0.20</u>	<u>-0.14</u>	-2.50
MgO	65.50	<u>-1.59</u>	-0.12	<u>-0.01</u>	5.27	*	-0.12	-4.61	0.24	-2.82	<u>0.39</u>	<u>0.56</u>	-3.21
CaO	56.60	<u>0.07</u>	0.00	<u>-1.32</u>	63.18	*	-1.32	0.00	<u>-12.64</u>	-1.32	<u>0.00</u>	<u>0.32</u>	-2.63
K <sub>2</sub> O	144.77	<u>-0.26</u>	-0.71	<u>0.17</u>	-9.38	*	0.11	-0.71	6.99	0.73	<u>0.61</u>	<u>-0.60</u>	-2.04
P <sub>2</sub> O <sub>5</sub>	*	0.35	0.00	<u>-2.35</u>	-1.74	*	-0.35	0.00	0.52	0.00	<u>0.00</u>	<u>-0.33</u>	0.00
LOI	<b>-4.80</b>	<u>0.44</u>	*	*	<b>10.66</b>	*	<b>12.08</b>	<u>1.86</u>	<b>11.19</b>	-0.72	<u>-0.05</u>	<u>-0.92</u>	<u>-2.89</u>
As	*	<u>-4.73</u>	*	<u>-1.01</u>	*	<b>2.10</b>	*	<b>6.27</b>	*	<u>-0.07</u>	<u>1.73</u>	*	*
Ba	*	<u>0.04</u>	*	<u>0.49</u>	3.26	0.97	<b>2.59</b>	<u>981.40</u>	0.41	-2.76	<u>-0.13</u>	<u>-4.66</u>	-2.04
Be	*	<u>1.76</u>	*	<u>4.67</u>	0.34	3.35	*	*	-0.30	*	*	*	*
Bi	*	<u>0.00</u>	*	<u>-0.64</u>	<u>-0.78</u>	9.90	*	*	*	<b>61.55</b>	*	*	*
Cd	*	<u>2.88</u>	*	<u>0.88</u>	-3.39	3.40	*	<b>88.93</b>	<u>0.77</u>	*	*	*	*
Ce	*	<u>-0.18</u>	*	<u>0.82</u>	2.54	0.06	*	0.67	0.40	-2.05	<u>0.00</u>	*	<u>-1.07</u>
Co	*	<u>-0.02</u>	*	<u>-0.06</u>	2.60	1.39	*	*	0.26	1.26	*	*	*
Cr	*	<u>-3.13</u>	*	<u>-0.55</u>	<u>-2.32</u>	-8.71	<u>-1.20</u>	-0.11	*	<u>-1.20</u>	<u>0.52</u>	<u>-0.37</u>	*
Cs	*	<u>0.49</u>	*	<u>0.32</u>	*	3.34	*	84.72	0.16	-3.51	*	*	<u>-0.06</u>
Cu	*	<u>1.56</u>	*	<u>-0.52</u>	<u>0.75</u>	0.13	<b>8.58</b>	<u>-2.90</u>	<u>-0.71</u>	-2.15	<u>-1.61</u>	*	<u>50.69</u>
Dy	*	<u>-2.23</u>	*	<u>1.10</u>	<u>-1.61</u>	1.09	*	*	<u>-1.10</u>	*	*	*	<u>-0.18</u>
Er	*	<u>-2.02</u>	*	<u>0.55</u>	<u>-0.29</u>	1.12	*	*	<u>-1.22</u>	*	*	*	*
Eu	*	<u>-0.52</u>	*	<u>0.96</u>	<u>-4.34</u>	-1.89	*	*	<u>-0.07</u>	*	*	*	*
Ga	*	<u>2.80</u>	*	<u>-0.74</u>	<u>0.90</u>	0.31	<u>-2.26</u>	<b>5.38</b>	*	<u>-2.26</u>	<u>-0.07</u>	*	*
Gd	*	<u>-0.43</u>	*	<u>0.36</u>	<u>-1.05</u>	0.16	*	*	<u>-0.57</u>	*	*	*	*
Hf	*	<u>-5.69</u>	*	<u>0.15</u>	*	<u>-12.64</u>	*	*	<u>-7.68</u>	<u>-0.21</u>	*	*	*
Ho	*	<u>-2.06</u>	*	<u>-0.16</u>	<u>-2.06</u>	-0.41	*	*	<u>-1.07</u>	*	*	*	*
La	*	<u>-0.39</u>	*	<u>0.68</u>	<u>0.58</u>	1.78	*	<u>-5.08</u>	-0.01	<u>-1.57</u>	<u>0.53</u>	*	<u>-1.43</u>
Li	*	<u>0.97</u>	*	<u>-0.48</u>	*	1.04	*	*	<b>0.83</b>	*	*	*	*
Lu	*	<u>-1.79</u>	*	<u>-0.88</u>	<u>0.72</u>	0.64	*	*	<u>-1.50</u>	*	*	*	*
Mo	*	<u>-0.71</u>	*	<u>-0.32</u>	<u>11.39</u>	-2.74	*	*	*	*	*	*	*
Nb	*	<u>-1.71</u>	*	<u>-0.13</u>	*	-5.87	*	0.08	2.88	<u>-0.57</u>	<u>0.36</u>	*	*
Nd	*	<u>-0.30</u>	*	<u>0.61</u>	<u>0.87</u>	0.70	*	1.70	0.46	<u>-2.69</u>	*	*	<u>-0.94</u>
Ni	*	<u>0.69</u>	*	<u>-0.60</u>	<u>2.18</u>	-0.67	*	<u>-2.40</u>	0.05	<u>-2.10</u>	<u>-0.54</u>	<u>0.78</u>	*
Pb	*	<u>0.20</u>	*	<u>-0.92</u>	<u>-8.98</u>	1.20	*	0.24	<u>-1.70</u>	<u>-0.89</u>	<u>0.36</u>	*	*
Pr	*	<u>-0.03</u>	*	<u>0.19</u>	<u>0.57</u>	<u>-0.25</u>	*	*	0.31	*	*	*	<u>0.86</u>
Rb	*	<u>-0.23</u>	*	<u>0.34</u>	<u>0.15</u>	1.91	<b>1.69</b>	<u>-2.66</u>	<u>-0.57</u>	<u>-0.84</u>	<u>0.42</u>	*	<u>-1.48</u>
Sb	*	<u>-0.21</u>	*	<u>-0.42</u>	<u>-11.13</u>	0.57	*	*	*	<u>-2.85</u>	*	*	*
Sc	*	<u>0.73</u>	*	*	<u>0.30</u>	2.52	*	<u>-3.64</u>	0.84	<u>-3.94</u>	<u>2.58</u>	*	*
Sm	*	<u>-0.36</u>	*	<u>-0.19</u>	<u>-0.77</u>	1.26	*	<u>-1.36</u>	0.15	3.17	*	*	*
Sn	*	<u>-2.69</u>	*	<u>-0.75</u>	*	0.14	*	<u>33.73</u>	<u>1.55</u>	<u>1.54</u>	*	*	*
Sr	*	<u>0.04</u>	*	<u>-0.82</u>	<u>2.05</u>	0.40	<u>-1.52</u>	<b>1.60</b>	0.45	<u>-0.76</u>	<u>0.38</u>	<u>1.84</u>	<u>-0.65</u>
Ta	*	<u>-1.05</u>	*	<u>-0.18</u>	*	<b>5.29</b>	*	*	<b>0.98</b>	<u>13.99</u>	*	*	*
Tb	*	<u>-1.15</u>	*	<u>-0.24</u>	<u>-4.93</u>	-0.37	*	*	<u>-0.56</u>	*	*	*	*
Th	*	<u>-0.43</u>	*	<u>11.13</u>	<u>-2.16</u>	-0.14	*	<b>4.42</b>	<u>-0.39</u>	<u>-2.30</u>	<u>0.25</u>	*	*
Tl	*	<u>-0.27</u>	*	<u>-0.02</u>	<u>0.47</u>	1.43	*	*	0.03	*	*	*	<u>0.75</u>
Tm	*	<u>-1.66</u>	*	<u>-0.44</u>	<u>-1.47</u>	1.33	*	*	<u>-1.47</u>	*	*	*	*
U	*	<u>-0.67</u>	*	<u>10.50</u>	<u>1.80</u>	-1.34	*	*	<u>-0.24</u>	<b>6.08</b>	<u>3.04</u>	*	<u>-0.42</u>
V	*	<u>-0.66</u>	*	<u>-0.74</u>	<u>1.06</u>	<u>-1.70</u>	<b>5.76</b>	<u>-1.51</u>	0.06	<u>-1.33</u>	<u>0.22</u>	<u>1.96</u>	*
W	*	<u>-1.37</u>	*	<u>-0.31</u>	*	-6.42	*	*	<u>-0.21</u>	<u>23.09</u>	*	*	*
Y	*	<u>-3.14</u>	*	<u>0.47</u>	<u>-1.41</u>	-0.93	*	<u>-0.76</u>	<u>-1.60</u>	<u>-1.95</u>	<u>0.11</u>	*	<u>-5.03</u>
Yb	*	<u>-2.03</u>	*	<u>0.93</u>	<u>-1.20</u>	-0.52	*	*	<u>-1.56</u>	<u>1.35</u>	*	*	*
Zn	*	<u>-0.13</u>	*	<u>0.24</u>	<u>-0.40</u>	-1.34	<u>-0.04</u>	<u>-5.55</u>	<u>-0.08</u>	<u>-0.77</u>	<u>-0.20</u>	<u>-0.62</u>	<u>27.51</u>
Zr	*	<u>-10.31</u>	*	<u>-1.58</u>	<u>-7.41</u>	<u>-22.86</u>	<u>-3.15</u>	<u>-1.42</u>	<u>-14.48</u>	<u>0.09</u>	<u>0.51</u>	<u>-0.28</u>	*

Bold entries are Data Quality 1 - Underlined entries are Data Quality 2 - Entries in italics are derived from Provisional Values.

Table 3 - GeoPT47A Z-scores for Silty soil, NES-1. 20/11/2020

Lab Code	J20	J21	J22	J24	J25	J26	J27	J28	J29	J30	J31	J33	J34
SiO <sub>2</sub>	-0.92	-0.30	-2.43	-0.01	0.29	-1.56	2.04	*	-0.19	-0.42	0.05	-0.57	-0.15
TiO <sub>2</sub>	-0.68	-0.74	-1.49	-0.33	-2.03	-1.02	2.03	-2.03	0.00	-0.95	-0.58	0.68	-0.20
Al <sub>2</sub> O <sub>3</sub>	-0.69	0.00	-0.92	0.40	0.11	-0.69	0.11	0.34	-2.69	-0.70	0.18	-0.46	0.16
Fe <sub>2</sub> O <sub>3T</sub>	2.26	1.12	-0.38	0.38	-0.40	-0.77	0.55	-0.97	1.61	-0.20	-0.68	2.18	-0.81
MnO	-0.40	0.36	-0.59	0.33	-0.40	-0.20	-0.40	-0.40	1.71	4.58	-0.39	1.33	0.18
MgO	-1.02	-1.02	-1.92	1.63	-1.02	-0.06	-2.82	-0.12	-0.51	0.61	0.84	0.39	1.47
CaO	0.00	0.00	0.00	-0.18	-1.32	17.11	-1.32	360.66	-1.32	-6.91	-1.18	3.29	1.12
K <sub>2</sub> O	-3.60	0.25	-1.19	0.62	-0.71	0.37	0.25	-1.68	1.09	0.37	0.20	0.13	-0.12
P <sub>2</sub> O <sub>5</sub>	0.00	-0.17	-1.05	0.26	0.00	-0.87	0.00	-1.74	-0.87	-0.09	9.76	0.61	-0.61
LOI	-0.54	2.04	6.84	-1.04	-1.52	8.00	*	*	3.55	0.52	0.53	2.13	1.75
As	0.28	*	0.28	-0.71	*	*	*	*	*	1.73	*	-2.59	*
Ba	-1.09	-0.42	-0.59	0.23	0.81	0.03	-0.42	-0.25	*	1.13	4.56	2.22	0.57
Be	0.00	*	0.17	0.18	3.78	*	*	1.51	*	*	*	*	*
Bi	0.00	*	*	1.41	0.21	*	*	1.41	*	*	*	*	*
Cd	0.04	*	1.22	-0.55	-0.99	*	*	-4.54	*	*	*	*	*
Ce	-0.31	0.32	2.00	-0.06	-1.15	-0.02	2.56	0.31	*	1.02	*	-0.51	*
Co	-0.09	*	1.00	0.30	0.00	0.25	-0.79	0.07	*	*	*	-0.91	*
Cr	2.66	0.30	5.05	-0.45	0.95	0.57	3.67	-0.07	*	0.71	1.46	-0.22	1.74
Cs	0.22	-0.28	*	0.39	-0.39	1.70	23.89	-0.00	*	*	*	*	*
Cu	2.36	1.07	0.54	0.32	1.08	-0.33	4.29	-0.43	*	-3.22	*	-0.54	-1.18
Dy	0.08	1.33	1.24	-0.15	0.00	-0.21	*	0.23	*	*	*	*	*
Er	-0.36	0.69	0.62	-0.09	0.13	-0.44	*	0.47	*	*	*	*	*
Eu	-0.02	0.87	0.00	-0.14	0.24	-0.35	*	0.00	*	*	*	*	*
Ga	0.54	-0.14	*	-0.02	-0.24	-0.06	6.23	0.07	*	0.99	*	-0.18	*
Gd	-0.30	0.40	2.86	-0.25	-0.25	0.28	*	-0.25	*	*	*	*	*
Hf	0.19	-1.12	1.59	-2.70	-3.10	-0.01	-8.67	-0.06	*	-1.16	*	4.12	*
Ho	0.43	1.13	0.56	-0.22	0.02	-0.09	*	0.00	*	*	*	*	*
La	-0.69	0.11	1.59	-0.13	-2.24	-0.29	4.58	0.01	82.65	1.41	*	-4.30	*
Li	0.58	*	1.84	-0.01	-0.22	*	*	0.07	*	*	*	*	*
Lu	-0.11	-0.36	0.72	-0.41	-0.36	-0.72	*	0.00	*	*	*	*	*
Mo	2.24	*	-2.58	-0.12	0.52	3.12	21.36	-0.25	*	*	*	*	*
Nb	-2.51	-0.80	0.21	0.06	-1.49	-0.12	4.61	0.47	*	2.30	*	-0.93	*
Nd	-0.28	0.18	0.87	-0.37	-0.56	-0.46	1.49	-0.28	85.40	-1.34	*	0.22	*
Ni	0.97	-4.14	1.58	0.70	-0.63	3.43	9.15	0.25	*	-1.05	*	-0.03	1.56
Pb	-0.48	-1.16	-0.24	-0.37	0.13	*	12.06	0.97	*	1.17	6.43	-0.44	4.37
Pr	-0.38	0.16	-0.25	-0.14	-0.47	-0.49	*	-0.06	*	*	*	*	*
Rb	0.25	-0.76	9.33	0.43	-2.70	0.72	3.80	0.00	*	-1.27	-0.42	-0.42	*
Sb	1.34	*	-1.09	1.21	0.42	0.62	*	*	*	*	*	*	*
Sc	0.76	-0.30	-0.42	0.58	0.05	0.00	11.22	0.73	*	*	*	1.82	*
Sm	-0.05	0.86	1.09	-0.29	0.13	-0.23	*	0.50	*	*	*	*	*
Sn	2.03	*	*	-0.14	-1.15	*	7.14	1.61	*	0.07	*	*	*
Sr	-0.15	0.76	0.23	0.78	-1.44	0.40	5.32	-0.84	*	*	0.00	-0.76	*
Ta	1.73	0.28	-1.17	-0.26	-0.98	-0.46	79.94	0.54	*	*	*	*	*
Tb	-0.27	1.28	0.08	-0.15	0.42	0.04	*	0.32	*	*	*	*	*
Th	0.00	0.20	1.35	-0.38	-0.14	-0.01	17.31	1.18	*	1.65	*	*	*
Tl	*	*	0.47	*	-0.83	*	*	1.46	*	*	*	*	*
Tm	-0.07	0.00	0.00	-0.45	0.00	-0.55	*	0.37	*	*	*	*	*
U	0.00	-0.13	0.74	-0.37	0.36	0.03	6.08	1.94	*	*	*	0.37	*
V	-2.08	0.00	4.61	0.68	-2.68	-0.13	-0.89	-2.22	17.06	3.99	*	0.00	11.81
W	1.07	*	*	0.00	0.13	*	11.19	-0.24	*	*	*	*	*
Y	-0.33	0.62	0.23	0.44	-0.27	-0.12	3.47	1.41	*	3.36	-2.06	-0.43	*
Yb	0.30	-0.08	1.36	-0.31	0.00	-0.60	*	0.68	*	*	*	*	*
Zn	1.38	0.69	-0.11	0.11	-0.91	0.72	3.61	-0.30	*	0.16	1.44	-1.11	2.39
Zr	0.37	-2.04	3.70	-3.56	-0.98	-0.91	0.93	2.41	*	2.18	0.19	-0.05	1.08

Bold entries are Data Quality 1 - Underlined entries are Data Quality 2 - Entries in italics are derived from Provisional Values.

Table 3 - GeoPT47A Z-scores for Silty soil, NES-1. 20/11/2020

Lab Code	J36	J37	J39	J40	J41	J42	J43	J45	J46	J49	J52	J54	J55
SiO <sub>2</sub>	0.30	<u>0.84</u>	-0.90	-0.53	-0.18	-0.09	<u>0.02</u>	-1.40	-1.39	-1.89	-0.63	-1.03	0.17
TiO <sub>2</sub>	1.35	<u>-0.27</u>	<u>-2.92</u>	<b>2.44</b>	<u>0.00</u>	0.47	<u>0.00</u>	-0.68	<b>2.03</b>	<u>0.07</u>	<u>-6.43</u>	0.68	0.68
Al <sub>2</sub> O <sub>3</sub>	-0.07	<u>0.86</u>	<u>-0.62</u>	<b>1.14</b>	-0.57	0.10	<u>0.80</u>	-0.46	-1.26	<u>12.02</u>	<u>0.52</u>	-1.60	1.60
Fe <sub>2</sub> O <sub>3T</sub>	0.76	<u>0.66</u>	<u>0.06</u>	<b>3.50</b>	<u>-0.87</u>	<u>0.91</u>	<u>1.99</u>	-0.48	<b>2.83</b>	<u>3.22</u>	<u>-3.43</u>	-1.16	0.93
MnO	1.90	<u>1.33</u>	<u>-0.87</u>	<b>3.50</b>	<u>-2.12</u>	<u>0.56</u>	<u>-3.95</u>	-0.20	<b>7.26</b>	<u>2.10</u>	<u>0.37</u>	3.43	-0.40
MgO	-2.19	<u>-3.21</u>	<u>-0.30</u>	<b>2.13</b>	<u>-0.51</u>	<u>-0.55</u>	<u>3.09</u>	-0.06	<b>18.76</b>	<u>7.76</u>	<u>-3.66</u>	0.78	-1.02
CaO	0.00	<u>1.32</u>	<u>-1.47</u>	<b>0.92</b>	<u>0.66</u>	<u>0.53</u>	<u>0.66</u>	-0.66	<b>73.71</b>	<u>3.49</u>	<u>-2.63</u>	1.32	3.95
K <sub>2</sub> O	0.01	<u>2.29</u>	<u>-0.24</u>	-0.81	<u>-1.56</u>	<u>-0.48</u>	<u>-0.36</u>	<u>1.09</u>	<u>0.73</u>	<u>3.26</u>	<u>-3.01</u>	0.25	-0.71
P <sub>2</sub> O <sub>5</sub>	-5.58	<u>0.00</u>	<u>-0.11</u>	<b>1.22</b>	<u>-0.70</u>	<u>0.17</u>	<u>1.66</u>	-0.44	*	<u>12.46</u>	*	0.00	-1.74
LOI	<u>0.04</u>	<u>-0.05</u>	*	<b>0.35</b>	<u>3.33</u>	<u>-0.45</u>	<u>-0.76</u>	<u>6.53</u>	<b>4.44</b>	*	<u>0.09</u>	<b>5.77</b>	<u>-3.03</u>
As	*	*	*	<b>6.98</b>	*	<u>-2.09</u>	<u>-0.12</u>	*	*	*	*	<u>1.73</u>	<b>6.63</b>
Ba	<u>1.32</u>	*	<u>-0.12</u>	<b>0.25</b>	*	<u>-0.35</u>	<u>-1.56</u>	*	*	<u>13.26</u>	*	<u>2.13</u>	<u>-1.42</u>
Be	*	*	*	*	*	<u>0.17</u>	*	*	*	*	*	*	*
Bi	*	*	*	*	*	*	*	*	*	*	*	*	*
Cd	*	*	*	*	*	*	*	*	*	*	*	*	*
Ce	<u>-2.15</u>	*	*	<b>3.07</b>	*	<u>0.04</u>	<u>-2.36</u>	*	<b>-0.72</b>	*	*	*	<b>2.56</b>
Co	<u>3.78</u>	*	*	<b>7.42</b>	*	<u>0.12</u>	<u>1.56</u>	*	*	*	*	*	<b>1.67</b>
Cr	<u>-2.43</u>	*	<u>-4.20</u>	<b>3.67</b>	*	<u>0.45</u>	<u>-1.78</u>	*	*	<u>2.77</u>	*	*	<u>-2.47</u>
Cs	<u>4.71</u>	*	*	*	*	<u>-0.47</u>	<u>-0.11</u>	*	*	*	*	*	<b>3.07</b>
Cu	<u>-1.45</u>	*	*	<b>5.37</b>	*	<u>-1.72</u>	<u>-0.54</u>	*	*	<u>45.61</u>	*	*	<u>-5.90</u>
Dy	<u>-1.93</u>	*	*	*	*	<u>0.22</u>	*	*	<b>-2.91</b>	*	*	*	*
Er	<u>-1.76</u>	*	*	*	*	<u>0.35</u>	*	*	<b>-5.55</b>	*	*	*	*
Eu	<u>-0.14</u>	*	*	*	*	<u>-0.09</u>	*	*	<b>-0.17</b>	*	*	*	*
Ga	<u>2.81</u>	*	*	<b>1.98</b>	*	<u>0.16</u>	<u>-1.24</u>	*	*	*	*	*	<u>-2.26</u>
Gd	<u>-1.33</u>	*	*	*	*	<u>-0.18</u>	*	*	<b>-0.45</b>	*	*	*	*
Hf	<u>-5.72</u>	*	*	*	*	<u>-0.18</u>	<u>1.69</u>	*	*	*	*	*	<u>-15.86</u>
Ho	<u>-1.73</u>	*	*	*	*	<u>0.09</u>	*	*	<b>-4.32</b>	*	*	*	*
La	<u>-2.59</u>	*	*	*	*	<u>0.22</u>	<u>-0.17</u>	*	<b>-1.48</b>	<u>11.95</u>	*	*	<b>13.18</b>
Li	<u>3.36</u>	*	*	*	*	<u>35.80</u>	*	*	*	*	*	*	*
Lu	<u>-2.02</u>	*	*	*	*	<u>0.00</u>	*	*	<b>-3.40</b>	*	*	*	*
Mo	*	*	*	*	*	<u>2.37</u>	*	*	*	*	*	*	*
Nb	<u>0.16</u>	*	*	<b>0.73</b>	<u>-0.28</u>	<u>-0.91</u>	<u>-0.48</u>	*	*	*	*	<b>2.02</b>	<u>-1.86</u>
Nd	<u>-1.83</u>	*	*	<b>-0.60</b>	*	<u>0.31</u>	<u>-0.45</u>	*	<b>-0.60</b>	<u>17.99</u>	*	*	<b>2.33</b>
Ni	<u>-0.87</u>	*	*	<b>1.99</b>	*	<u>-1.30</u>	<u>-1.41</u>	*	*	<u>9.18</u>	*	*	<u>-2.10</u>
Pb	<u>-1.86</u>	*	*	<b>-0.89</b>	*	<u>-0.46</u>	<u>-0.97</u>	*	*	*	*	*	<b>16.59</b>
Pr	<u>-1.91</u>	*	*	*	*	<u>0.25</u>	*	*	<b>-1.27</b>	*	*	*	*
Rb	<u>-0.55</u>	*	*	<b>2.53</b>	<u>1.90</u>	<u>-0.07</u>	<u>-0.74</u>	*	*	<u>1.06</u>	*	<b>1.69</b>	<u>-0.84</u>
Sb	*	*	*	*	*	*	<u>17.88</u>	*	*	*	*	*	*
Sc	<u>9.40</u>	*	*	*	*	<u>-0.30</u>	<u>-2.12</u>	*	*	*	*	*	<b>10.01</b>
Sm	<u>-0.77</u>	*	*	*	*	<u>0.25</u>	<u>4.31</u>	*	<b>-0.50</b>	*	*	*	<b>4.08</b>
Sn	*	*	*	*	*	<u>0.00</u>	<u>9.52</u>	*	*	*	*	*	*
Sr	<u>1.59</u>	*	*	<b>3.80</b>	<u>2.66</u>	<u>-0.27</u>	<u>-0.57</u>	*	*	<u>3.04</u>	*	<u>1.90</u>	<u>-0.76</u>
Ta	<u>-0.12</u>	*	*	*	*	<u>-0.26</u>	*	*	*	*	*	*	*
Tb	<u>-1.16</u>	*	*	*	*	<u>-0.32</u>	*	*	<b>0.56</b>	*	*	*	*
Th	<u>-0.42</u>	*	*	*	*	<u>-0.03</u>	<u>-2.55</u>	*	<b>-0.53</b>	*	*	*	<u>-5.66</u>
Tl	*	*	*	*	*	<u>-1.10</u>	*	*	*	*	*	*	*
Tm	<u>-1.79</u>	*	*	*	*	<u>0.00</u>	*	*	<b>-0.74</b>	*	*	*	*
U	<u>1.14</u>	*	*	*	*	<u>0.23</u>	<u>1.04</u>	*	<b>-0.60</b>	*	*	*	<b>4.75</b>
V	<u>1.51</u>	*	<u>0.60</u>	<b>3.10</b>	<u>-1.99</u>	<u>-1.88</u>	<u>-2.39</u>	*	*	*	*	*	<u>0.44</u>
W	*	*	*	*	*	*	<u>5.00</u>	*	*	*	*	*	<u>90.92</u>
Y	<u>2.38</u>	*	*	<b>1.30</b>	<u>-2.60</u>	<u>0.00</u>	<u>-0.60</u>	*	<b>-7.37</b>	*	*	<u>-0.87</u>	<u>0.00</u>
Yb	<u>-1.47</u>	*	*	*	*	<u>0.11</u>	<u>-3.08</u>	*	<b>-5.11</b>	*	*	*	*
Zn	<u>-0.30</u>	*	<u>0.64</u>	<b>1.78</b>	*	<u>-0.40</u>	<u>-1.24</u>	*	*	<u>-1.66</u>	<u>0.12</u>	<u>-0.02</u>	<u>-1.06</u>
Zr	<u>-1.47</u>	*	<u>-9.84</u>	<u>0.56</u>	<u>-0.65</u>	<u>0.32</u>	<u>-0.01</u>	*	*	<u>0.93</u>	*	<u>-0.55</u>	<u>-0.46</u>

Bold entries are Data Quality 1 - Underlined entries are Data Quality 2 - Entries in italics are derived from Provisional Values.

Table 3 - GeoPT47A Z-scores for Silty soil, NES-1. 20/11/2020

Lab Code	J56	J57	J59	J60	J61	J62	J64	J65	J67	J68	J69	J70	J71
SiO <sub>2</sub>	<b>0.49</b>	<b>-1.00</b>	<b>-0.08</b>	<b>0.21</b>	<b>-0.76</b>	-1.03	-0.13	0.01	<b>-0.37</b>	<b>0.18</b>	*	*	-0.09
TiO <sub>2</sub>	<b>0.34</b>	<b>-2.03</b>	<b>0.34</b>	<b>2.71</b>	<b>2.03</b>	0.00	0.00	0.11	<b>-0.69</b>	<b>0.00</b>	0.24	-4.13	<b>0.00</b>
Al <sub>2</sub> O <sub>3</sub>	<b>0.74</b>	<b>-0.34</b>	<b>0.80</b>	<b>-0.40</b>	<b>2.58</b>	-1.83	-3.21	-0.34	<b>-0.10</b>	<b>0.34</b>	-2.22	-3.09	<b>-0.40</b>
Fe <sub>2</sub> O <sub>3T</sub>	<b>-0.01</b>	<b>2.37</b>	<b>0.09</b>	<b>-0.20</b>	<b>4.93</b>	-1.35	0.93	2.28	<b>-0.08</b>	<b>0.93</b>	0.00	-1.35	<b>-0.39</b>
MnO	<b>3.63</b>	<b>1.71</b>	<b>-2.12</b>	<b>-0.20</b>	<b>-0.20</b>	-1.55	0.36	1.01	<b>0.05</b>	<b>-0.40</b>	0.28	-1.55	<b>-1.35</b>
MgO	<b>-1.41</b>	<b>2.19</b>	<b>0.84</b>	<b>-1.86</b>	<b>1.29</b>	-1.56	-8.21	-1.38	<b>0.29</b>	<b>-0.12</b>	0.96	-1.47	<b>1.74</b>
CaO	<b>0.00</b>	<b>3.29</b>	<b>-0.66</b>	<b>0.00</b>	<b>3.29</b>	<b>17.37</b>	<b>-1.32</b>	<b>-1.58</b>	<b>0.23</b>	<b>2.63</b>	<b>1.97</b>	<b>-1.58</b>	<b>5.27</b>
K <sub>2</sub> O	<b>0.61</b>	<b>-0.84</b>	<b>0.37</b>	<b>-0.60</b>	<b>0.13</b>	<b>0.39</b>	<b>-0.23</b>	<b>0.73</b>	<b>0.00</b>	<b>0.25</b>	<b>-1.03</b>	<b>-0.71</b>	<b>-2.04</b>
P <sub>2</sub> O <sub>5</sub>	<b>0.00</b>	<b>-0.87</b>	<b>0.00</b>	<b>0.00</b>	<b>-6.97</b>	<b>20.56</b>	<b>-0.52</b>	<b>-0.12</b>	<b>-0.58</b>	<b>1.74</b>	<b>-0.78</b>	<b>-2.44</b>	<b>-1.22</b>
LOI	<b>2.75</b>	*	<b>-0.18</b>	<b>0.53</b>	<b>-0.18</b>	<b>8.53</b>	<b>-0.98</b>	<b>-1.07</b>	<b>0.18</b>	<b>0.26</b>	<b>8.20</b>	*	<b>-0.18</b>
As	<b>0.85</b>	*	*	*	*	*	<b>0.00</b>	<b>-2.10</b>	*	*	*	*	*
Ba	<b>-0.13</b>	<b>1.71</b>	*	*	<b>-0.29</b>	-0.08	1.25	-0.13	*	<b>4.93</b>	<b>0.20</b>	<b>-0.17</b>	<b>0.38</b>
Be	*	*	*	*	*	<b>0.20</b>	<b>-0.18</b>	*	*	*	*	*	<b>0.92</b>
Bi	*	*	*	*	*	*	<b>1.98</b>	<b>1.06</b>	*	*	*	*	*
Cd	*	*	*	*	*	<b>-0.34</b>	<b>0.96</b>	<b>-3.32</b>	*	*	*	*	*
Ce	<b>2.82</b>	<b>0.00</b>	*	*	*	<b>0.23</b>	<b>0.51</b>	<b>0.50</b>	*	<b>3.07</b>	*	<b>-0.50</b>	<b>0.41</b>
Co	<b>-2.45</b>	<b>3.71</b>	*	*	<b>-0.40</b>	<b>0.26</b>	<b>-0.52</b>	*	*	*	*	<b>-0.40</b>	<b>0.53</b>
Cr	<b>-0.60</b>	<b>-0.97</b>	*	*	<b>-7.15</b>	<b>1.61</b>	<b>0.30</b>	<b>4.34</b>	*	<b>21.63</b>	<b>1.22</b>	<b>-1.85</b>	<b>0.15</b>
Cs	*	*	*	*	*	0.38	0.45	0.47	*	*	*	-0.77	<b>0.46</b>
Cu	<b>1.07</b>	<b>2.15</b>	*	*	<b>-3.22</b>	-0.79	-0.72	2.98	*	<b>2.15</b>	<b>-0.36</b>	<b>0.45</b>	<b>-0.38</b>
Dy	*	<b>-2.37</b>	*	*	*	-0.31	-3.82	0.51	*	*	*	-0.21	<b>-0.11</b>
Er	*	<b>-2.70</b>	*	*	*	-0.06	-0.20	0.50	*	*	*	-0.81	<b>-0.14</b>
Eu	*	<b>0.17</b>	*	*	*	-0.35	<b>-0.29</b>	0.33	*	*	*	-0.66	<b>0.26</b>
Ga	<b>2.05</b>	*	*	*	<b>4.17</b>	<b>-1.05</b>	<b>1.57</b>	<b>0.09</b>	*	<b>6.23</b>	*	<b>-0.14</b>	<b>0.35</b>
Gd	*	<b>-2.83</b>	*	*	*	-0.30	<b>0.50</b>	<b>0.98</b>	*	*	*	1.00	<b>0.33</b>
Hf	*	*	*	*	*	<b>-0.08</b>	<b>0.85</b>	<b>0.40</b>	*	*	*	<b>0.45</b>	<b>-0.42</b>
Ho	*	<b>-2.06</b>	*	*	*	0.08	<b>-0.66</b>	<b>0.26</b>	*	*	*	-0.34	<b>-0.09</b>
La	<b>-0.35</b>	<b>1.41</b>	*	*	*	-0.35	<b>-1.41</b>	<b>-0.09</b>	*	<b>8.09</b>	*	-0.77	<b>0.14</b>
Li	*	<b>-0.11</b>	*	*	*	<b>0.57</b>	<b>1.07</b>	*	*	*	*	<b>0.02</b>	<b>0.83</b>
Lu	*	<b>0.18</b>	*	*	*	-0.39	<b>-0.25</b>	<b>-0.07</b>	*	*	*	-0.86	<b>-0.18</b>
Mo	*	*	*	*	*	0.37	<b>1.95</b>	1.88	*	*	*	0.18	<b>-0.04</b>
Nb	<b>0.36</b>	*	*	*	<b>-2.22</b>	<b>0.65</b>	<b>3.39</b>	<b>0.45</b>	*	<b>0.73</b>	*	<b>0.14</b>	<b>-0.22</b>
Nd	*	<b>-0.30</b>	*	*	*	-0.24	<b>-1.10</b>	<b>0.56</b>	*	<b>4.63</b>	*	<b>-0.54</b>	<b>0.43</b>
Ni	<b>0.49</b>	<b>2.02</b>	*	*	<b>-0.54</b>	<b>-0.62</b>	<b>-0.09</b>	<b>2.57</b>	*	<b>34.72</b>	<b>1.90</b>	<b>0.51</b>	<b>-0.13</b>
Pb	<b>0.77</b>	<b>1.98</b>	*	*	<b>1.17</b>	-1.45	-0.72	<b>-1.45</b>	*	<b>-0.08</b>	*	<b>-0.79</b>	<b>-0.53</b>
Pr	*	<b>1.52</b>	*	*	*	0.13	<b>-1.23</b>	<b>1.16</b>	*	*	*	-0.25	<b>0.44</b>
Rb	<b>0.21</b>	<b>-0.63</b>	*	*	*	-0.04	<b>1.48</b>	<b>0.03</b>	*	<b>0.84</b>	*	<b>-0.76</b>	<b>-0.04</b>
Sb	*	*	*	*	*	<b>1.55</b>	<b>4.00</b>	<b>18.24</b>	*	*	*	*	<b>0.50</b>
Sc	<b>-0.45</b>	<b>-0.45</b>	*	*	<b>7.13</b>	<b>0.52</b>	<b>1.92</b>	<b>1.49</b>	*	*	<b>1.46</b>	<b>0.18</b>	<b>0.08</b>
Sm	*	<b>0.68</b>	*	*	*	-0.09	<b>-0.53</b>	<b>0.16</b>	*	*	*	-0.23	<b>0.36</b>
Sn	*	*	*	*	*	3.29	<b>4.70</b>	<b>2.66</b>	*	*	*	*	<b>1.47</b>
Sr	<b>0.00</b>	<b>0.00</b>	*	*	<b>8.74</b>	-0.15	-0.99	0.46	*	<b>6.08</b>	<b>0.91</b>	<b>-0.66</b>	<b>0.49</b>
Ta	*	*	*	*	*	0.37	<b>2.39</b>	<b>3.22</b>	*	*	*	0.28	<b>0.60</b>
Tb	*	<b>-1.99</b>	*	*	*	-0.08	<b>1.45</b>	<b>0.66</b>	*	*	*	<b>0.78</b>	<b>0.04</b>
Th	*	<b>-1.15</b>	*	*	*	-0.92	<b>0.38</b>	<b>0.39</b>	*	<b>0.50</b>	*	<b>-0.34</b>	<b>0.06</b>
Tl	*	*	*	*	*	0.00	<b>0.00</b>	1.23	*	*	*	*	<b>-0.10</b>
Tm	*	<b>-1.47</b>	*	*	*	0.00	<b>-0.59</b>	<b>0.18</b>	*	*	*	0.00	<b>-0.18</b>
U	*	<b>-0.30</b>	*	*	*	-0.03	<b>0.40</b>	<b>0.46</b>	*	*	*	-0.53	<b>-0.10</b>
V	<b>1.99</b>	<b>0.89</b>	*	*	<b>5.09</b>	<b>-1.48</b>	<b>-0.35</b>	<b>0.18</b>	*	<b>-2.22</b>	<b>0.66</b>	<b>-1.87</b>	<b>-0.73</b>
W	*	*	*	*	*	<b>0.36</b>	<b>6.83</b>	*	*	*	*	*	<b>-0.18</b>
Y	<b>0.11</b>	<b>-3.52</b>	*	*	<b>3.36</b>	-0.76	1.17	1.12	*	<b>1.30</b>	<b>5.06</b>	<b>0.03</b>	<b>-0.33</b>
Yb	*	<b>-1.58</b>	*	*	*	0.14	<b>-0.58</b>	<b>0.48</b>	*	*	*	-0.08	<b>-0.19</b>
Zn	<b>-1.11</b>	<b>1.44</b>	*	*	<b>0.16</b>	-0.77	-1.02	4.81	*	<b>-1.13</b>	<b>0.68</b>	-2.27	<b>-1.02</b>
Zr	<b>-0.18</b>	<b>-2.18</b>	*	*	<b>-1.48</b>	1.11	-0.28	1.44	<b>-14.91</b>	1.67	*	3.02	<b>-0.09</b>

Bold entries are Data Quality 1 - Underlined entries are Data Quality 2 - Entries in italics are derived from Provisional Values.

Table 3 - GeoPT47A Z-scores for Silty soil, NES-1. 20/11/2020

Lab Code	J72	J73	J74	J75	J76	J77	J79	J80	J81	J82	J83	J84	J85
SiO <sub>2</sub>	-0.75	-0.45	1.50	-0.33	0.10	-1.29	0.13	0.30	-0.13	-0.51	-0.63	*	-0.66
TiO <sub>2</sub>	*	0.34	0.47	0.34	0.00	1.83	-0.07	0.00	0.68	3.15	-1.02	*	0.37
Al <sub>2</sub> O <sub>3</sub>	*	3.61	1.69	-0.52	0.17	5.32	0.08	0.34	0.00	3.66	-0.40	*	0.34
Fe <sub>2</sub> O <sub>3T</sub>	*	0.75	1.05	-0.20	-0.01	1.51	0.28	0.36	-0.39	1.13	-0.48	*	0.85
MnO	*	0.56	3.04	-0.20	*	4.39	0.37	3.43	-0.97	-0.78	-0.20	*	0.76
MgO	*	6.23	-4.16	-0.96	-0.06	-15.34	-0.01	3.48	0.39	*	-0.51	*	-0.96
CaO	*	1.32	-5.40	-0.66	-0.66	7.90	-0.59	3.95	-0.66	21.46	-1.32	*	0.66
K <sub>2</sub> O	*	1.33	0.78	0.13	-0.12	2.29	0.27	-0.71	-0.60	-0.36	-0.36	*	0.13
P <sub>2</sub> O <sub>5</sub>	*	-0.44	-0.52	-0.87	1.74	2.79	-0.09	0.00	0.00	*	0.00	*	0.00
LOI	0.49	-0.18	-1.34	0.53	-1.38	5.06	0.06	-1.25	0.98	*	6.62	*	-0.36
As	*	-0.04	*	*	0.19	7.28	-1.91	*	*	-1.09	0.23	6.98	*
Ba	*	-0.21	-1.75	0.38	-1.13	3.30	0.21	-1.17	0.46	*	0.00	2.59	1.00
Be	*	1.00	-10.03	*	-0.25	-0.92	-0.33	-0.17	*	*	-0.42	-0.84	*
Bi	*	*	*	*	-0.71	3.18	2.48	*	*	*	0.00	-2.83	*
Cd	*	-0.36	-1.10	*	-0.78	0.21	0.02	*	*	*	-0.36	0.80	*
Ce	*	-0.26	-3.14	*	1.02	3.84	0.74	-0.05	*	*	-0.26	1.89	-0.23
Co	*	0.72	-2.29	*	-0.12	2.27	-0.02	0.03	*	*	0.02	2.64	*
Cr	*	-1.35	9.66	-2.10	-1.44	1.83	-0.04	-0.15	*	-0.88	-0.41	1.09	*
Cs	*	*	-1.92	*	-0.25	1.81	-0.93	-0.22	-1.67	*	-0.30	2.35	*
Cu	*	0.27	-2.96	*	-0.46	3.00	-0.18	0.00	0.00	0.11	0.97	19.96	*
Dy	*	-2.50	-6.59	*	0.39	-0.88	2.46	0.23	*	*	-2.27	-0.71	-0.13
Er	*	-2.48	-6.23	*	0.50	-1.08	1.14	-0.14	*	*	-0.29	-1.19	0.08
Eu	*	-0.69	-2.43	*	0.09	0.26	-0.26	0.35	*	*	0.35	-0.17	-0.09
Ga	*	0.59	-2.39	2.05	-0.86	3.17	-0.80	0.07	*	*	-0.10	6.44	*
Gd	*	-1.25	-2.31	*	0.10	-0.08	2.23	-0.15	*	*	-1.23	1.00	-0.45
Hf	*	*	*	*	-5.60	-2.33	0.47	-0.21	-2.54	*	-5.60	-7.89	-1.38
Ho	*	-2.16	-5.63	*	0.19	-0.94	1.03	-0.38	*	*	-1.97	-1.50	0.00
La	*	-0.61	-3.03	-1.22	0.40	1.59	3.65	-0.52	*	*	0.22	1.41	-0.30
Li	*	-0.01	-2.45	*	-0.29	-0.20	-1.04	-0.96	*	*	-0.53	-2.17	*
Lu	*	-1.79	-5.01	*	-0.18	-1.07	0.00	0.36	*	*	-1.25	-2.50	0.00
Mo	*	0.12	-1.41	*	-0.54	12.34	0.79	-0.25	*	*	0.71	6.90	*
Nb	*	1.01	-5.02	*	-1.22	4.70	-0.52	0.08	*	*	0.49	2.15	-2.92
Nd	*	-0.40	-2.78	*	0.85	1.43	1.17	-0.28	*	*	0.64	1.08	-0.15
Ni	*	0.49	-2.81	-0.54	-0.77	3.30	-0.18	0.46	-0.33	*	0.33	2.91	*
Pb	*	0.08	-3.68	*	0.00	1.78	-1.58	0.00	*	-3.11	0.12	1.13	*
Pr	*	-0.40	-0.41	*	0.66	1.36	-0.09	-0.44	*	*	0.02	1.36	-0.27
Rb	*	0.27	-2.65	*	-0.27	1.69	-0.53	-0.30	*	-0.17	-0.32	2.36	-0.32
Sb	*	-0.27	-1.20	*	-0.32	2.99	0.23	*	*	*	1.22	7.52	*
Sc	*	-0.68	-1.94	-0.45	-0.27	3.34	*	-0.30	*	*	-0.45	0.67	0.00
Sm	*	-0.39	-2.18	*	0.57	0.91	-0.77	0.00	*	*	0.88	0.77	0.00
Sn	*	-0.80	*	*	-0.84	4.27	10.88	0.84	*	*	-0.98	1.47	-1.33
Sr	*	-0.11	-2.10	-0.76	-0.04	4.26	0.19	-0.46	0.00	-1.37	0.34	3.12	0.27
Ta	*	*	*	*	-1.11	8.32	-0.26	-0.51	*	*	0.40	7.40	-0.26
Tb	*	-1.63	-3.74	*	0.28	-0.91	-0.20	0.80	*	*	-0.32	-0.87	0.40
Th	*	*	7716.81	*	0.15	1.79	0.43	-0.06	-2.06	*	0.07	0.59	-0.45
Tl	*	0.40	-1.86	*	-0.65	0.90	*	-0.53	*	*	0.40	-0.53	*
Tm	*	-1.84	-5.16	*	0.00	-0.92	0.00	0.74	*	*	-0.18	-2.58	0.00
U	*	-0.30	-3.34	*	-0.57	1.37	1.34	0.07	*	*	-0.30	-0.13	0.37
V	*	0.47	-4.08	-0.44	-0.97	2.88	-1.99	-1.15	*	*	-1.55	3.50	1.02
W	*	*	*	*	-1.15	20.47	0.83	*	*	*	-1.55	15.71	*
Y	*	0.65	-9.82	*	0.33	-1.57	-0.92	0.43	*	*	-0.16	-1.73	0.00
Yb	*	-2.37	-6.09	*	0.56	-1.24	1.43	-0.15	*	*	0.23	-1.28	-0.08
Zn	*	0.51	2.50	-0.93	-0.37	-1.30	0.20	-0.40	-0.02	0.07	0.53	-1.24	*
Zr	*	-0.09	-1.10	*	-10.45	-3.33	0.51	0.36	0.05	-0.41	-0.05	-13.70	-1.59

Bold entries are Data Quality 1 - Underlined entries are Data Quality 2 - Entries in italics are derived from Provisional Values.

Table 3 - GeoPT47A Z-scores for Silty soil, NES-1. 20/11/2020


Lab Code	J87	J88	J89	J91	J95	J96	J99	J100	J101	J102	J103	J105	J106
SiO <sub>2</sub>	-18.66	<u>-0.02</u>	-5.58	-0.14	-0.76	0.11	1.23	*	0.09	-16.44	0.15	-0.63	0.00
TiO <sub>2</sub>	-1.90	-0.14	-2.03	1.35	-1.90	0.24	4.06	*	0.00	6.09	1.79	-1.35	0.47
Al <sub>2</sub> O <sub>3</sub>	-4.12	0.06	10.76	2.12	2.29	0.17	-2.18	*	0.06	106.14	-0.23	-1.83	-0.26
Fe <sub>2</sub> O <sub>3T</sub>	-3.99	0.37	-1.53	3.98	5.88	0.28	-1.16	*	1.61	59.49	0.75	-0.02	-0.27
MnO	0.75	0.56	9.56	3.24	3.69	0.18	-2.32	*	-0.20	22.57	0.18	3.43	-0.91
MgO	2.85	<u>-0.06</u>	*	3.99	-1.38	0.52	-1.02	*	-0.06	158.99	1.38	-11.80	0.52
CaO	-1.45	1.32	1.45	2.63	-3.95	-0.07	0.00	*	-0.66	13.16	-0.53	-3.95	-0.46
K <sub>2</sub> O	0.06	-0.12	1.33	1.33	0.83	0.61	-39.25	*	0.13	83.11	0.37	-4.09	-0.07
P <sub>2</sub> O <sub>5</sub>	-0.17	-0.26	*	1.74	2.44	-0.52	6.97	*	0.00	-10.46	-0.17	-10.46	*
LOI	*	0.22	*	0.75	5.56	-0.89	3.37	*	-0.27	-15.07	0.58	11.02	1.20
As	*	*	-0.74	*	*	1.29	*	*	2.78	24.60	*	*	*
Ba	*	<u>-0.88</u>	-0.38	-0.46	0.55	0.05	*	5.37	-0.01	43.74	*	*	*
Be	*	*	*	*	0.52	2.68	*	4.20	2.01	*	*	*	*
Bi	*	*	*	*	*	*	*	0.92	0.00	*	*	*	*
Cd	*	*	*	*	*	*	*	*	0.59	*	*	*	*
Ce	*	*	-0.15	*	0.00	0.05	*	4.46	0.28	19.25	*	*	*
Co	*	*	*	-0.70	0.46	-0.22	*	2.31	0.10	*	*	*	*
Cr	*	2.58	1.20	0.71	-6.37	-0.82	*	3.58	-2.64	25.75	*	*	*
Cs	*	*	*	*	1.28	0.60	*	1.13	*	20.05	*	*	*
Cu	*	0.54	2.79	1.61	-0.24	-0.38	*	1.18	1.02	23.61	*	*	*
Dy	*	*	*	*	-4.25	0.17	*	0.18	0.19	13.34	*	*	*
Er	*	*	*	*	-4.58	0.46	*	-0.00	0.42	9.49	*	*	*
Eu	*	*	*	*	-0.87	0.09	*	1.79	0.09	15.96	*	*	*
Ga	*	2.05	*	1.42	-0.20	0.78	*	3.92	0.79	*	*	*	*
Gd	*	*	*	*	-2.01	0.10	*	1.82	0.35	16.00	*	*	*
Hf	*	0.42	*	*	-10.78	0.26	*	-6.18	-1.30	-4.40	*	*	*
Ho	*	*	*	*	27.77	0.09	*	0.08	0.19	9.20	*	*	*
La	*	*	-1.14	*	-0.30	0.45	*	3.38	-0.13	10.28	*	*	*
Li	*	*	*	*	1.76	*	*	2.80	-1.13	*	*	*	*
Lu	*	*	*	*	-3.44	0.36	*	-0.75	-0.18	5.01	*	*	*
Mo	*	*	*	*	-0.62	*	*	3.91	-0.12	5.40	*	*	*
Nb	*	<u>-2.22</u>	2.89	1.66	-1.55	-0.10	*	1.57	-2.94	0.57	*	*	*
Nd	*	*	0.22	*	-0.39	-0.10	*	3.44	0.12	16.49	*	*	*
Ni	*	1.00	*	0.49	-0.00	0.18	*	2.02	1.35	62.33	*	*	*
Pb	*	*	1.30	2.39	0.91	0.49	*	3.18	-0.28	9.95	*	*	*
Pr	*	*	*	*	0.13	0.00	*	2.12	-0.06	12.75	*	*	*
Rb	*	-1.27	0.49	*	1.27	0.21	*	7.29	-0.25	18.99	*	*	*
Sb	*	*	*	*	*	*	*	1.16	1.50	*	*	*	*
Sc	*	*	*	0.15	0.30	*	*	2.97	-0.11	37.57	*	*	*
Sm	*	*	*	*	-0.41	0.14	*	2.21	0.36	16.01	*	*	*
Sn	*	*	*	*	*	*	*	-3.30	0.14	*	*	*	*
Sr	*	1.14	0.08	1.14	0.38	0.23	*	5.00	0.00	31.18	*	*	*
Ta	*	*	*	*	-2.24	1.13	*	1.60	-1.91	0.94	*	*	*
Tb	*	*	*	*	-2.54	0.40	*	1.09	0.28	12.51	*	*	*
Th	*	*	-1.01	*	0.66	0.36	*	2.01	-0.66	10.89	*	*	*
Tl	*	*	*	*	*	*	*	*	-0.10	*	*	*	*
Tm	*	*	*	*	*	0.18	*	-0.66	0.18	6.27	*	*	*
U	*	*	<u>-2.21</u>	*	-1.07	0.47	*	0.12	0.67	7.42	*	*	*
V	*	<u>-0.44</u>	*	<u>-0.22</u>	-0.76	0.17	*	0.52	-0.86	31.01	*	*	*
W	*	*	*	*	-5.00	23.80	*	*	-2.32	*	*	*	*
Y	*	0.65	-2.76	1.19	-5.75	0.24	*	0.63	-0.49	17.01	*	*	*
Yb	*	*	*	*	-3.98	0.38	*	-0.29	0.04	8.72	*	*	*
Zn	*	0.71	-1.11	1.80	0.04	0.18	*	2.27	0.16	16.74	*	*	*
Zr	*	0.37	-1.23	1.57	-19.64	0.82	*	-8.76	-0.22	-8.10	*	*	*

Bold entries are Data Quality 1 - Underlined entries are Data Quality 2 - Entries in italics are derived from Provisional Values.


Table 3 - GeoPT47A Z-scores for Silty soil, NES-1. 20/11/2020

Lab Code	J108	J109	J112	J116	J117	J118	J120	J121	J122	J123	J124	J126	J128
SiO <sub>2</sub>	<b>0.39</b>	0.76	0.15	-0.33	-0.10	0.17	0.37	-0.07	-0.70	0.06	-0.68	-4.01	0.59
TiO <sub>2</sub>	-0.34	<b>0.00</b>	0.34	0.00	1.22	0.00	<b>2.71</b>	0.00	0.30	-1.35	-0.61	0.17	-2.03
Al <sub>2</sub> O <sub>3</sub>	<b>0.92</b>	<b>0.00</b>	0.52	-0.11	-0.06	0.06	-0.34	0.97	0.69	0.57	-0.01	-0.46	0.11
Fe <sub>2</sub> O <sub>3T</sub>	-0.29	-1.35	0.56	-0.48	0.02	-0.20	1.12	0.37	-0.67	-0.59	0.66	0.19	0.93
MnO	*	*	-0.24	-2.12	-0.01	-0.20	3.43	0.01	-0.01	-0.40	0.87	0.37	-0.40
MgO	-0.51	-1.02	0.39	-0.51	-0.60	-0.06	-1.02	0.03	-1.86	2.58	0.97	0.48	2.58
CaO	-1.32	<b>0.00</b>	0.66	0.00	-0.59	-0.66	<b>7.90</b>	1.78	-0.66	22.38	-3.36	0.66	-2.63
K <sub>2</sub> O	-0.60	0.25	-0.12	0.13	-2.43	0.13	-2.16	1.06	0.61	-1.19	-0.21	0.13	0.25
P <sub>2</sub> O <sub>5</sub>	-0.87	5.23	0.00	0.00	0.00	0.00	-1.74	-0.70	0.00	0.00	-0.52	-0.09	0.00
LOI	<b>-1.25</b>	<b>0.62</b>	*	<b>2.58</b>	0.11	-1.29	<b>3.46</b>	-1.29	<b>1.15</b>	3.28	*	*	-3.56
As	*	*	<b>-1.48</b>	*	*	-0.04	*	*	<b>1.73</b>	-0.60	*	*	1.69
Ba	*	*	<b>0.29</b>	*	<b>-0.71</b>	-0.38	<b>6.94</b>	-0.54	-1.13	3.18	*	<b>0.63</b>	<b>7.28</b>
Be	*	*	<b>2.59</b>	*	*	0.75	*	*	<b>0.17</b>	-0.17	*	*	*
Bi	*	*	<b>0.00</b>	*	*	-0.35	*	*	*	*	*	*	*
Cd	*	*	<b>0.59</b>	*	*	-0.55	*	*	-0.36	*	*	*	*
Ce	*	*	<b>0.31</b>	*	<b>-0.33</b>	0.49	*	*	-1.33	-0.61	*	<b>0.26</b>	<b>2.56</b>
Co	*	*	<b>0.04</b>	*	*	-0.09	<b>7.42</b>	*	<b>0.63</b>	2.29	*	*	-11.06
Cr	*	*	<b>1.72</b>	*	*	1.27	<b>2.92</b>	-0.41	-0.04	0.00	<b>0.15</b>	<b>1.27</b>	-0.07
Cs	*	*	<b>0.74</b>	*	<b>-0.06</b>	-0.11	*	*	<b>0.27</b>	-0.77	*	*	40.33
Cu	*	*	<b>-0.48</b>	*	*	0.00	<b>5.37</b>	2.68	1.07	0.64	*	<b>3.76</b>	-5.37
Dy	*	*	<b>0.64</b>	*	<b>-0.31</b>	-0.13	*	*	<b>-3.20</b>	-0.76	*	*	*
Er	*	*	<b>0.16</b>	*	<b>-0.07</b>	-0.07	*	*	<b>-3.08</b>	-0.89	*	*	*
Eu	*	*	<b>0.17</b>	*	<b>-0.35</b>	1.04	*	*	<b>-0.78</b>	0.35	*	*	*
Ga	*	*	<b>0.15</b>	*	<b>0.08</b>	-0.60	*	*	<b>-3.25</b>	-0.78	*	*	<b>4.10</b>
Gd	*	*	<b>0.43</b>	*	<b>-0.35</b>	0.00	*	*	<b>-2.31</b>	0.85	*	*	0.35
Hf	*	*	<b>0.91</b>	*	<b>0.14</b>	-0.32	*	*	<b>-3.28</b>	<b>0.00</b>	*	*	<b>8.25</b>
Ho	*	*	<b>0.09</b>	*	<b>-0.19</b>	0.75	*	*	<b>-2.63</b>	-0.38	*	*	*
La	*	*	<b>0.14</b>	*	<b>-0.35</b>	0.05	<b>8.97</b>	*	<b>-1.44</b>	-0.25	*	<b>0.53</b>	<b>6.33</b>
Li	*	*	<b>0.13</b>	*	*	-0.81	*	*	<b>-0.34</b>	*	*	*	*
Lu	*	*	<b>0.18</b>	*	<b>-0.36</b>	0.18	*	*	<b>-2.50</b>	<b>0.36</b>	*	*	*
Mo	*	*	<b>0.46</b>	*	*	-0.12	<b>752.87</b>	*	<b>0.04</b>	1.41	*	*	*
Nb	*	*	<b>-0.02</b>	*	<b>-0.93</b>	-0.15	<b>5.90</b>	*	<b>0.36</b>	-0.83	*	*	4.61
Nd	*	*	<b>-0.09</b>	*	<b>-0.30</b>	0.17	*	*	<b>-1.24</b>	-0.70	*	*	1.49
Ni	*	*	<b>0.74</b>	*	*	-0.03	<b>8.13</b>	*	<b>-1.05</b>	-0.77	*	<b>2.53</b>	<b>5.06</b>
Pb	*	*	<b>0.32</b>	*	*	-0.04	<b>8.01</b>	<b>2.79</b>	<b>-0.04</b>	0.73	*	*	1.54
Pr	*	*	<b>0.11</b>	*	<b>-0.13</b>	0.25	*	*	<b>-0.85</b>	<b>0.19</b>	*	*	*
Rb	*	*	<b>0.08</b>	*	<b>-0.53</b>	-0.36	<b>9.71</b>	<b>0.00</b>	<b>0.21</b>	-0.89	*	*	<b>2.53</b>
Sb	*	*	<b>0.95</b>	*	*	<b>-0.32</b>	*	*	<b>-0.71</b>	*	*	*	*
Sc	*	*	<b>0.96</b>	*	*	<b>-0.45</b>	*	*	<b>0.15</b>	-0.30	*	*	<b>8.19</b>
Sm	*	*	<b>0.45</b>	*	<b>0.00</b>	0.00	*	*	<b>-0.91</b>	-0.45	*	*	*
Sn	*	*	<b>0.49</b>	*	*	-1.33	*	*	<b>-1.33</b>	<b>-0.56</b>	*	*	*
Sr	*	*	<b>0.23</b>	*	<b>-0.15</b>	0.68	<b>12.93</b>	<b>4.18</b>	<b>-0.08</b>	3.12	<b>-0.38</b>	*	<b>-0.76</b>
Ta	*	*	<b>1.06</b>	*	<b>0.20</b>	<b>0.40</b>	*	*	*	<b>4.76</b>	*	*	*
Tb	*	*	<b>0.28</b>	*	<b>-0.20</b>	<b>0.40</b>	*	*	<b>-2.11</b>	<b>0.80</b>	*	*	*
Th	*	*	<b>0.46</b>	*	<b>-0.11</b>	-0.17	<b>31.31</b>	*	<b>-0.90</b>	<b>0.22</b>	*	*	<b>-5.10</b>
Tl	*	*	<b>0.23</b>	*	*	-0.27	*	*	<b>-0.43</b>	*	*	*	*
Tm	*	*	<b>0.18</b>	*	<b>0.00</b>	0.37	*	*	<b>-2.40</b>	<b>0.74</b>	*	*	*
U	*	*	<b>0.40</b>	*	<b>0.33</b>	<b>0.70</b>	<b>52.87</b>	*	<b>-1.04</b>	<b>0.07</b>	*	*	<b>-0.60</b>
V	*	*	<b>0.42</b>	*	*	<b>-0.66</b>	<b>3.99</b>	<b>1.11</b>	<b>0.44</b>	-0.93	*	<b>0.00</b>	<b>3.99</b>
W	*	*	<b>0.30</b>	*	*	*	*	*	*	<b>1.67</b>	*	*	*
Y	*	*	<b>0.65</b>	*	<b>-0.54</b>	-0.11	<b>6.72</b>	*	<b>0.65</b>	<b>0.76</b>	*	<b>-0.43</b>	<b>3.47</b>
Yb	*	*	<b>0.45</b>	*	<b>-0.38</b>	0.19	*	*	<b>-3.12</b>	<b>-0.15</b>	*	*	*
Zn	*	*	<b>0.44</b>	*	*	0.16	<b>8.35</b>	-0.75	-0.38	-4.23	<b>0.16</b>	<b>0.16</b>	<b>1.42</b>
Zr	<b>0.37</b>	*	<b>-0.28</b>	*	<b>0.23</b>	-0.09	<b>6.48</b>	<b>0.28</b>	<b>-2.41</b>	<b>2.66</b>	*	<b>-0.05</b>	<b>-2.41</b>


Bold entries are Data Quality 1 - Underlined entries are Data Quality 2 - Entries in italics are derived from Provisional Values.

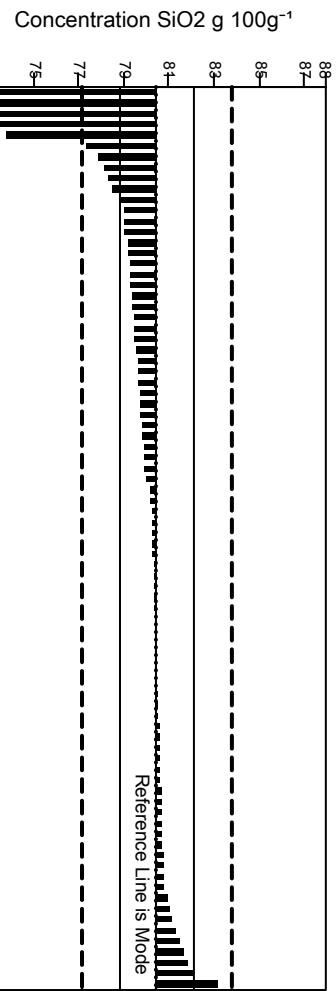


GeoPT47A - Barchart for Al2O3

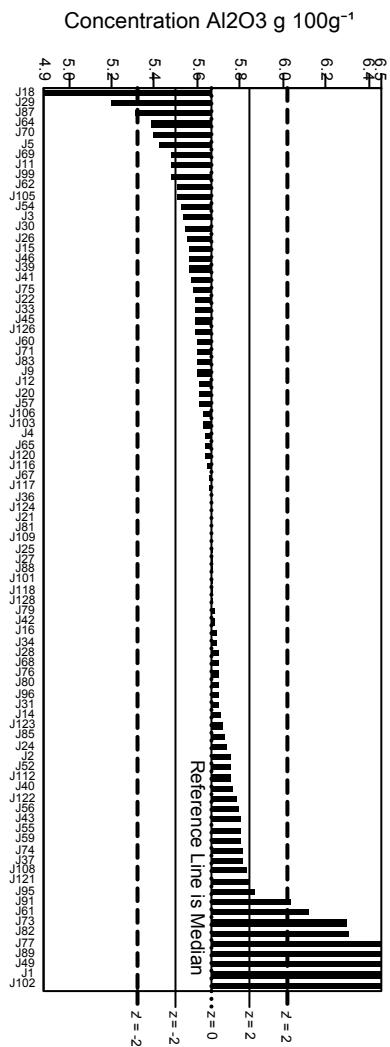


### Concentration Fe<sub>2</sub>O<sub>3</sub>T g 100g<sup>-1</sup>

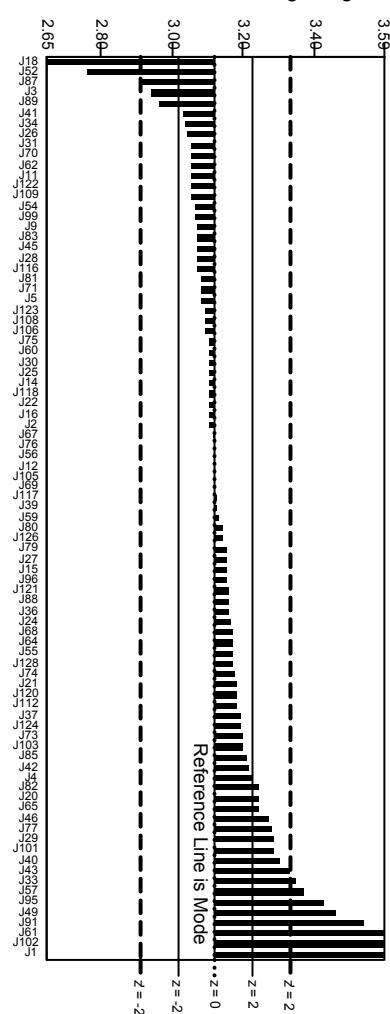

Geopt47A - Barchart for MgC

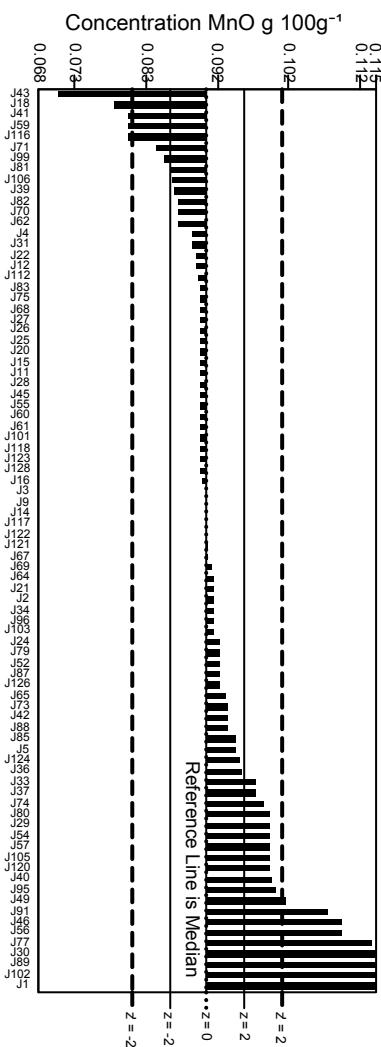

GeoPT47A - Barchart for MnO

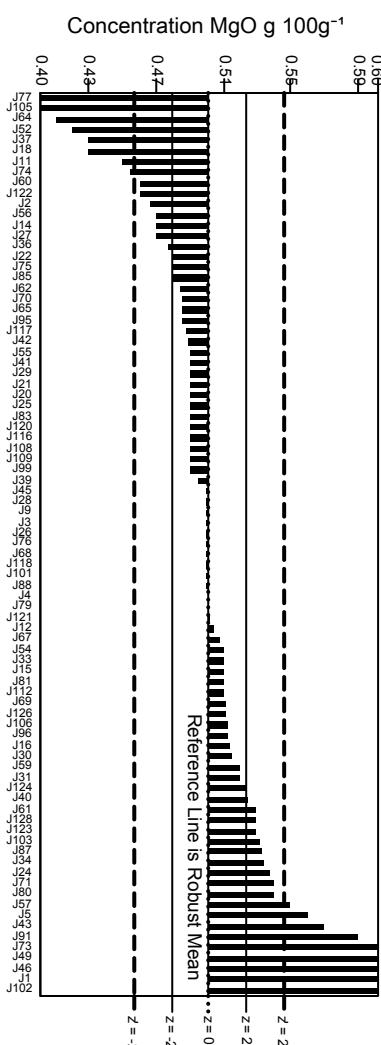


Concentration  $\text{TiO}_2 \text{ g } 100\text{g}^{-1}$

Reference Line is Median

$z = -2$


$z = 2$

## GeoPT47A - Barchart for CaO

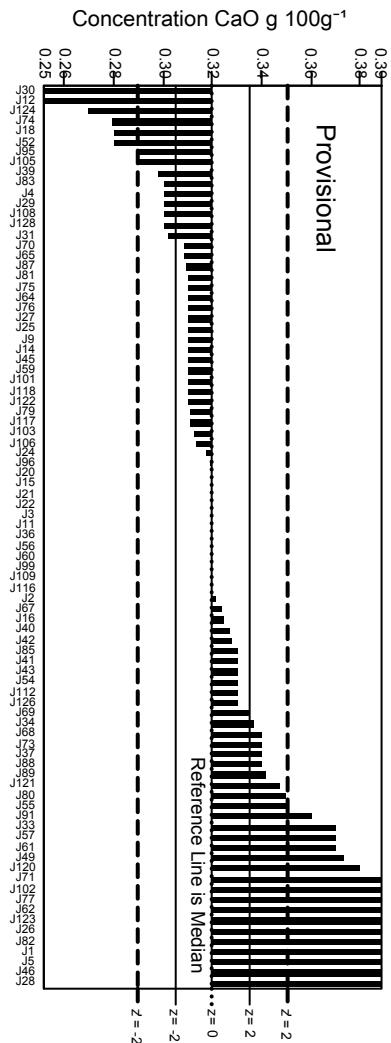


GeoPT47A - Barchart for CaO

## GeoPT47A - Barchart for K2O

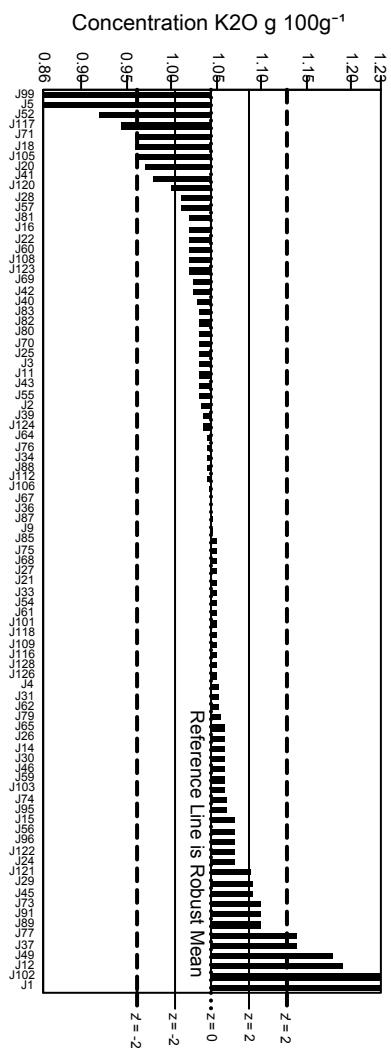


GeoPT47A - Barchart for K2O

## GeoPT47A - Barchart for P2O5

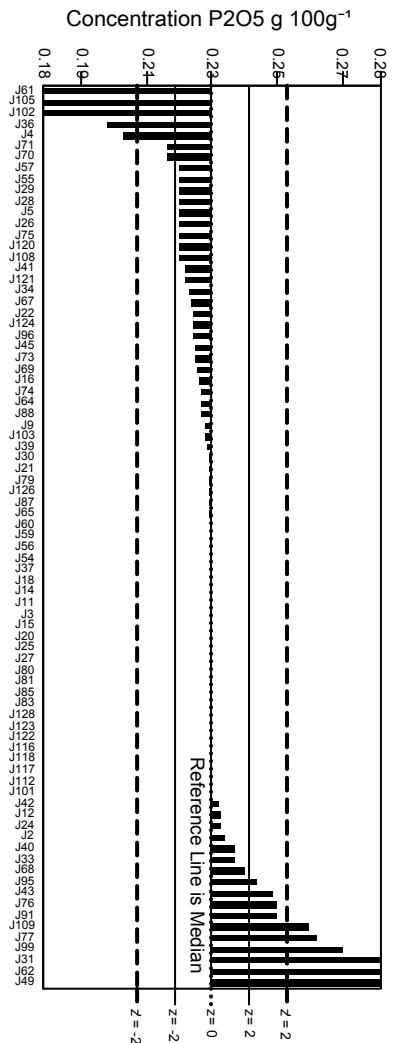


GeoPT47A - Barchart for P2O5

## GeoPT47A - Barchart for As

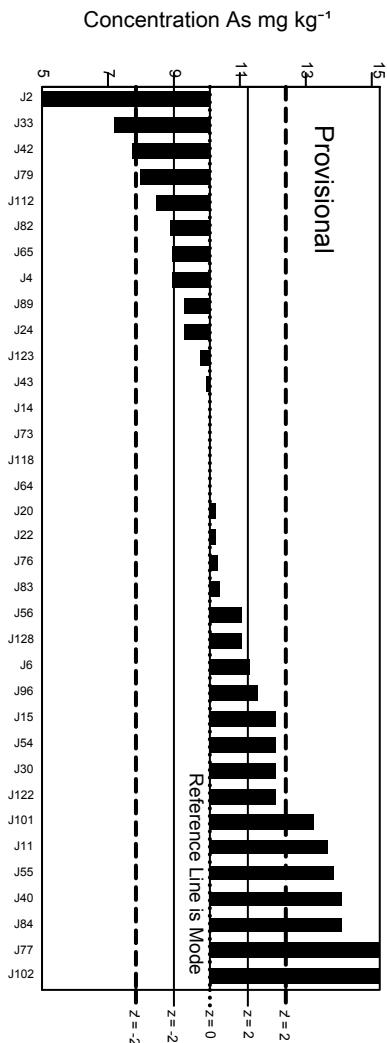


GeoPT47A - Barchart for As

## GeoPT47A - Barchart for LOI

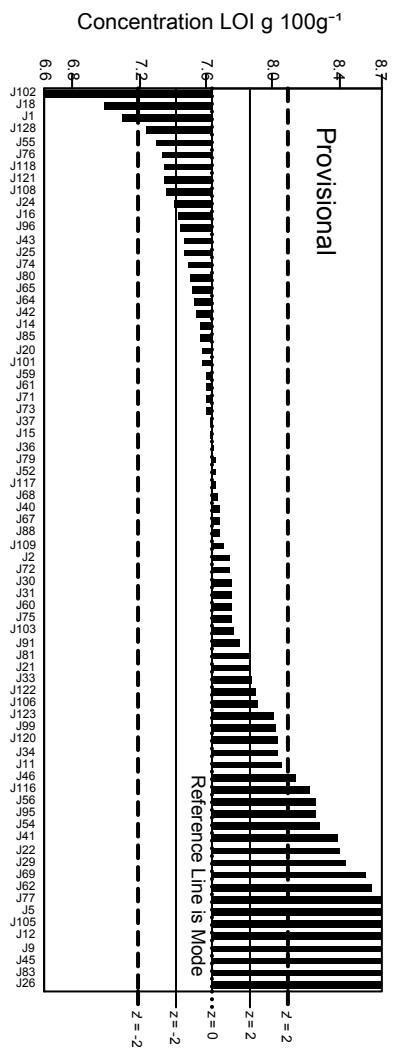



GeoPT47A - Barchart for LOI

## GeoPT47A - Barchart for Ba

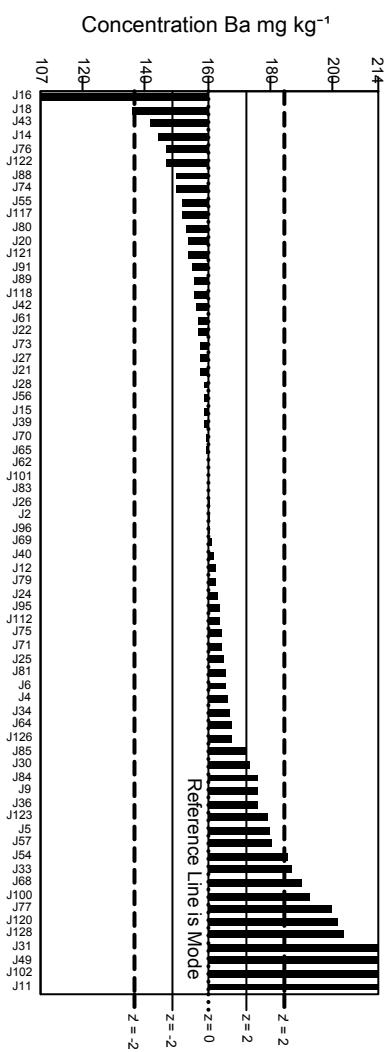


GeoPT47A - Barchart for Ba


### GeoPT47A - Barchart for Be

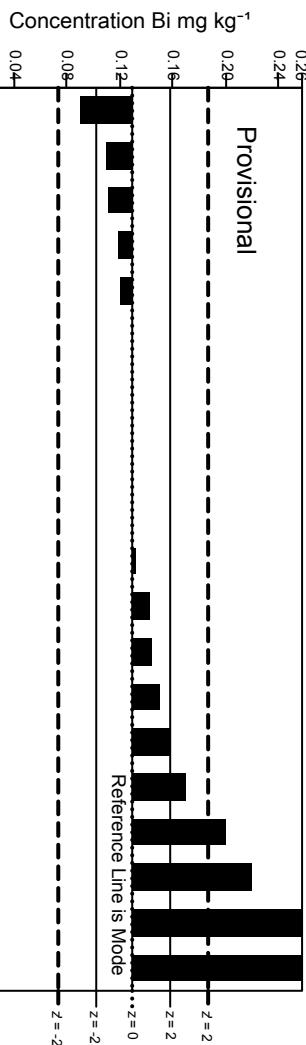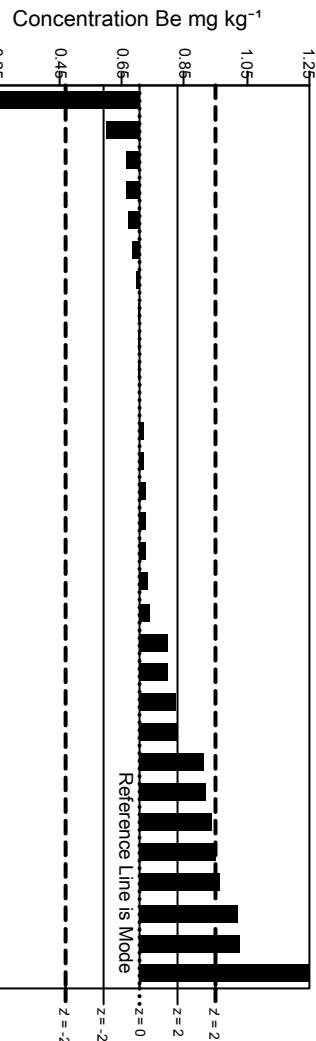


### GeoPT47A - Barchart for Cd

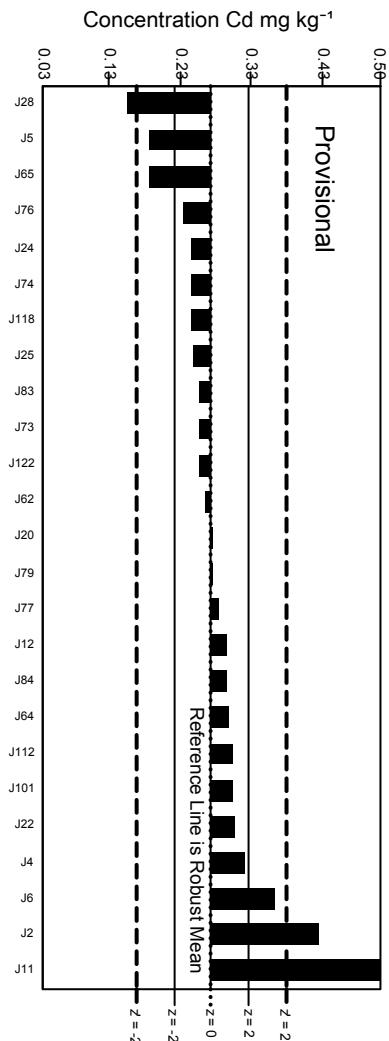


### GeoPT47A - Barchart for Co

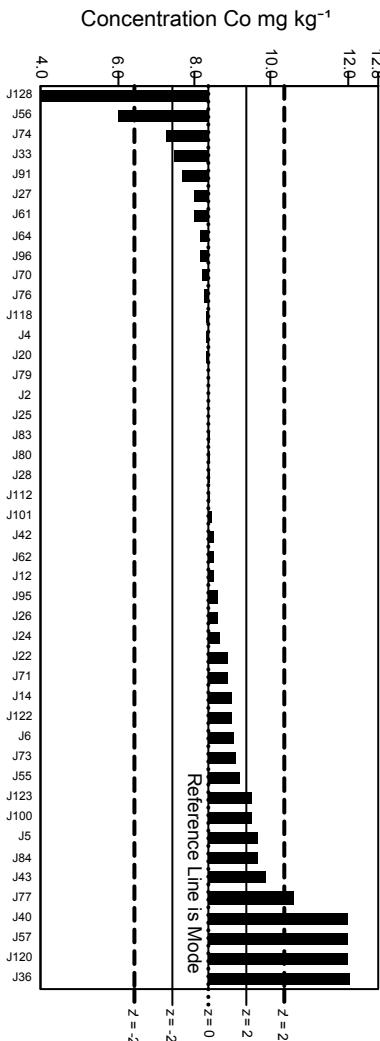


### Concentration Ce $\text{mg kg}^{-1}$

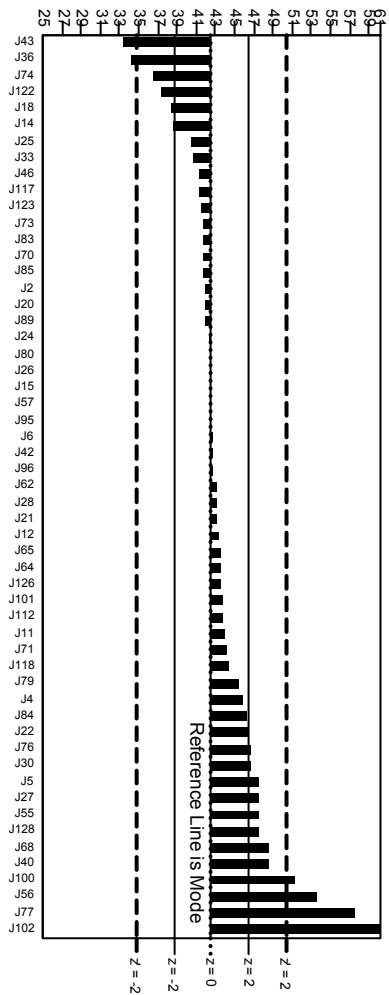


### GeoPT47A - Barchart for Cr

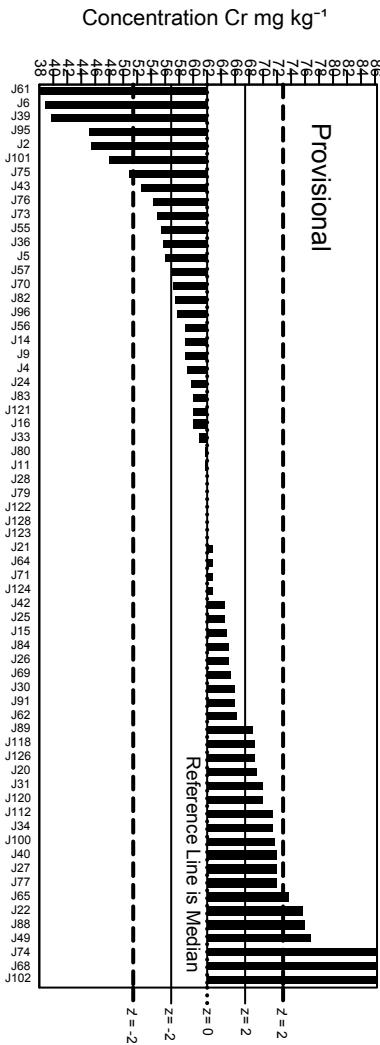


### GeoPT47A - Barchart for Cs

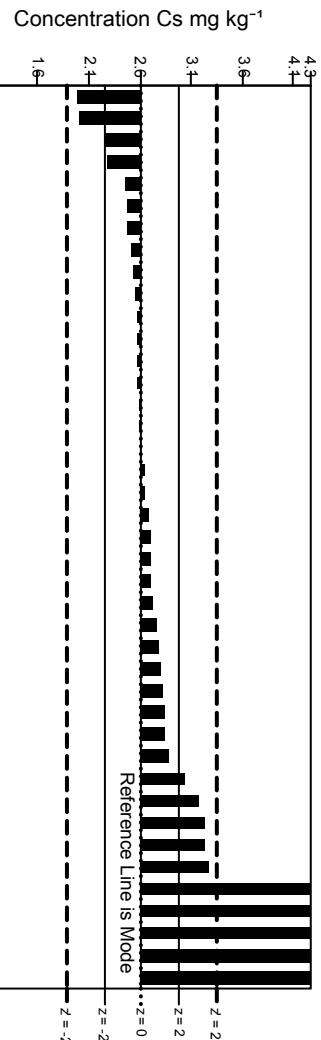


### GeoPT47A - Barchart for Cu

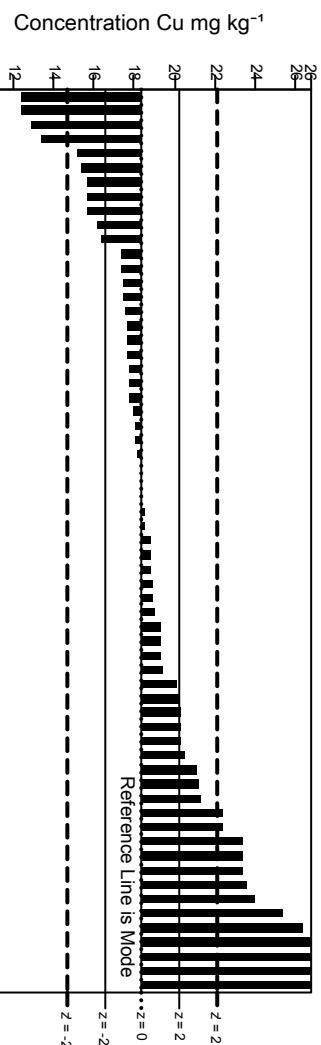


### GeoPT47A - Barchart for Dy

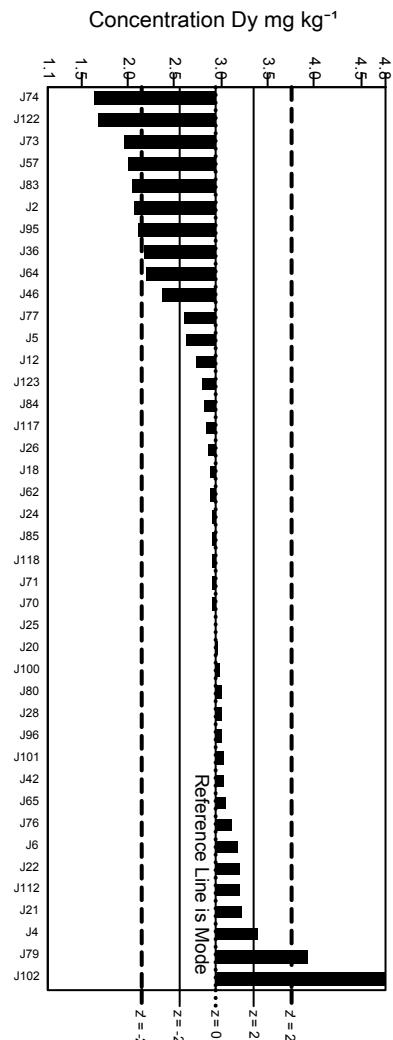


### GeoPT47A - Barchart for Er

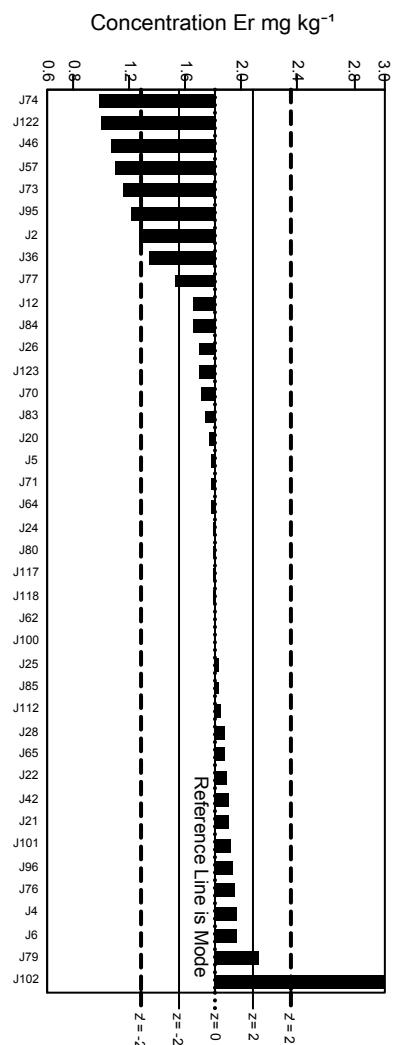


### GeoPT47A - Barchart for Eu

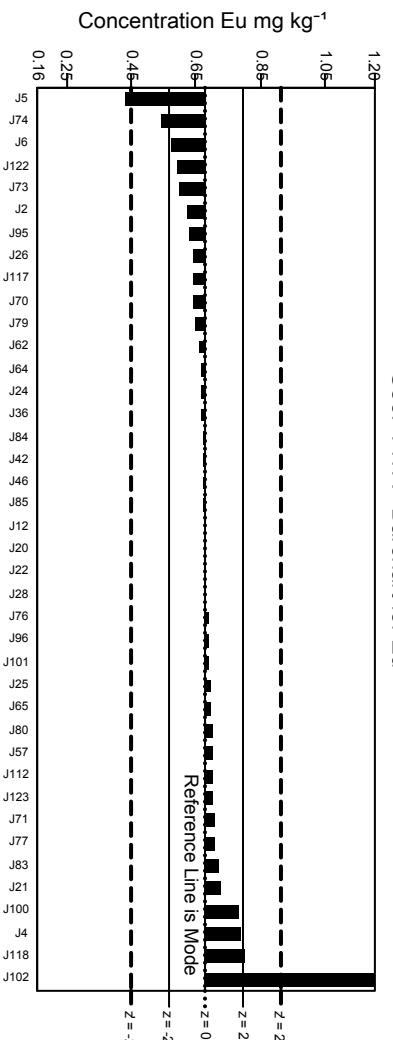


### GeoPT47A - Barchart for Ga

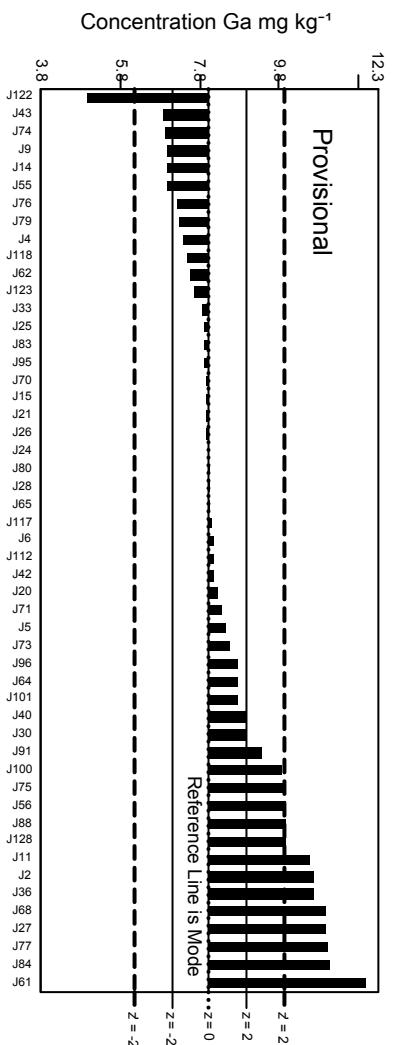


## GeoPT47A - Barchart for Gd

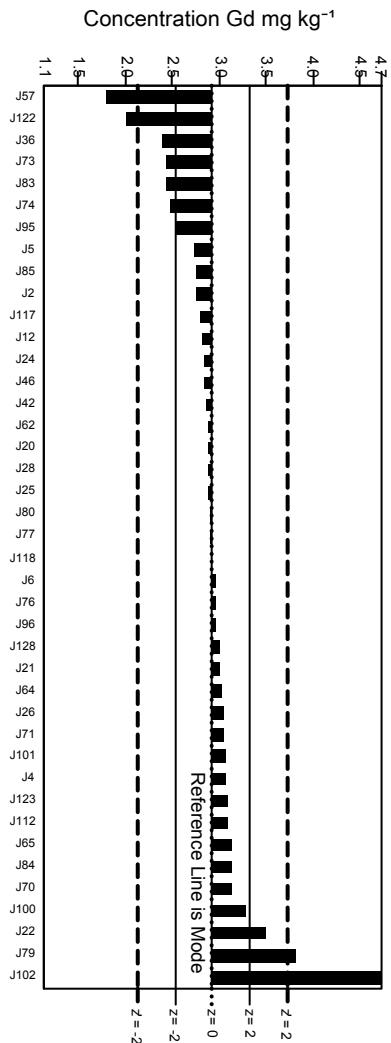


## GeoPT47A - Barchart for Hf

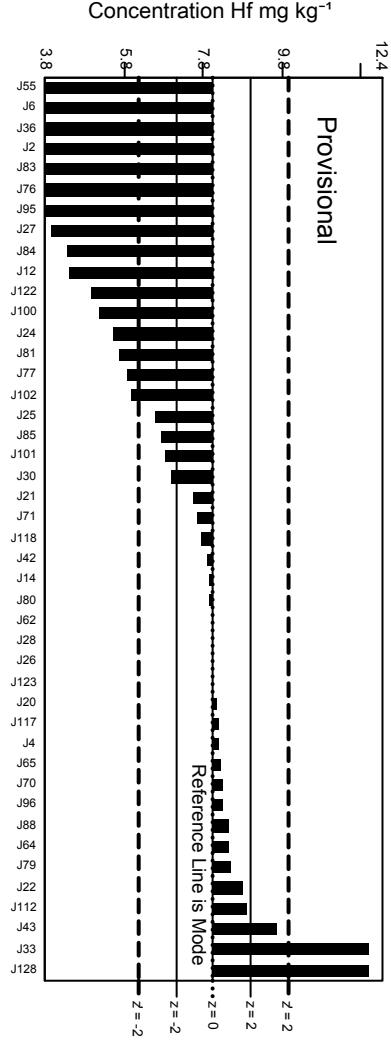


## GeoPT47A - Barchart for Ho

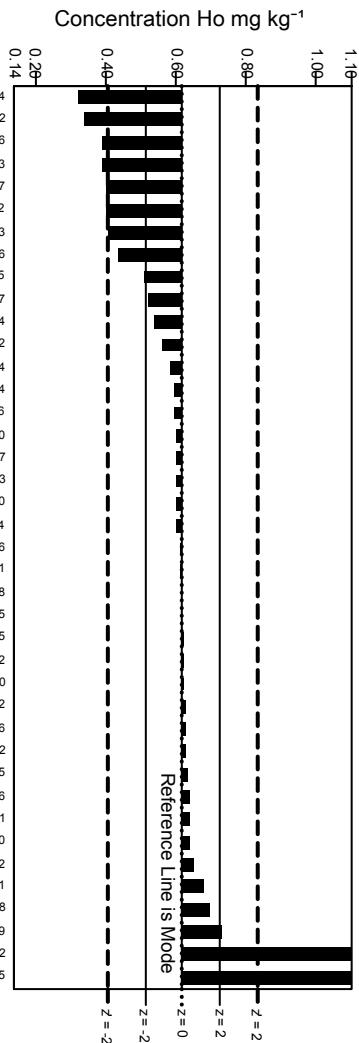


## GeoPT47A - Barchart for Li

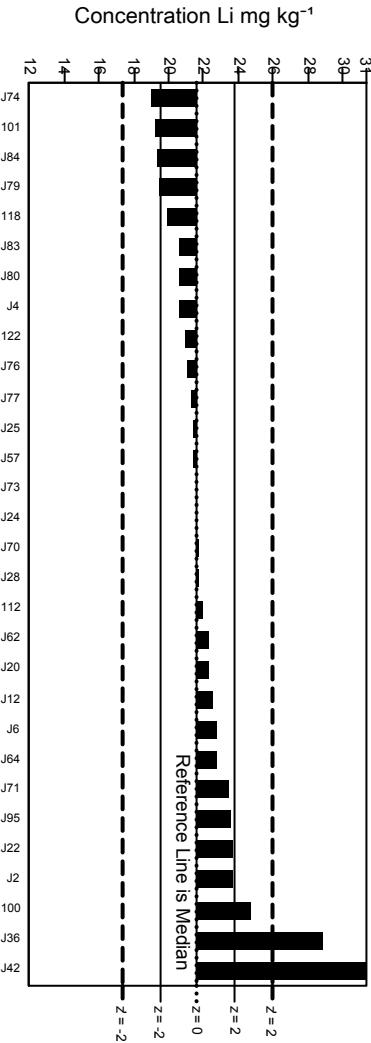






## GeoPT47A - Barchart for Lu

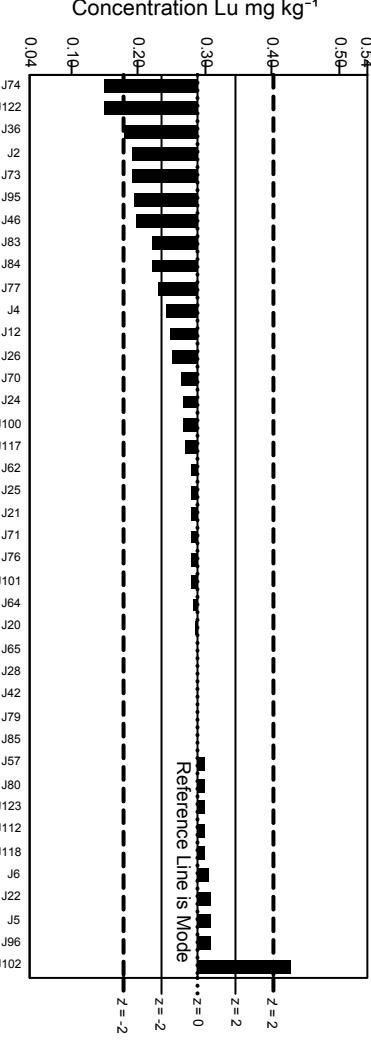


## GeoPT47A - Barchart for Mo

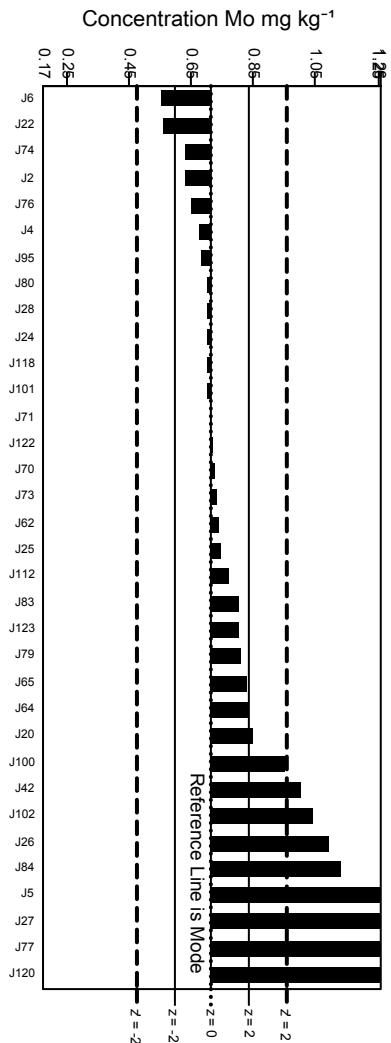


## GeoPT47A - Barchart for Nb

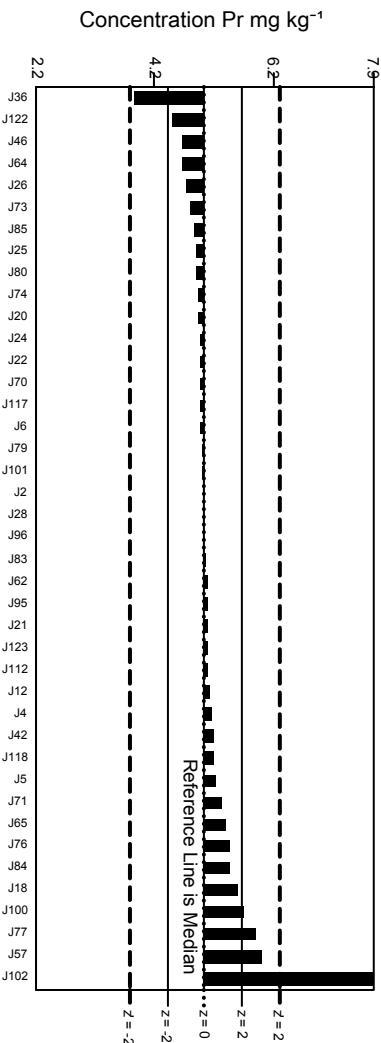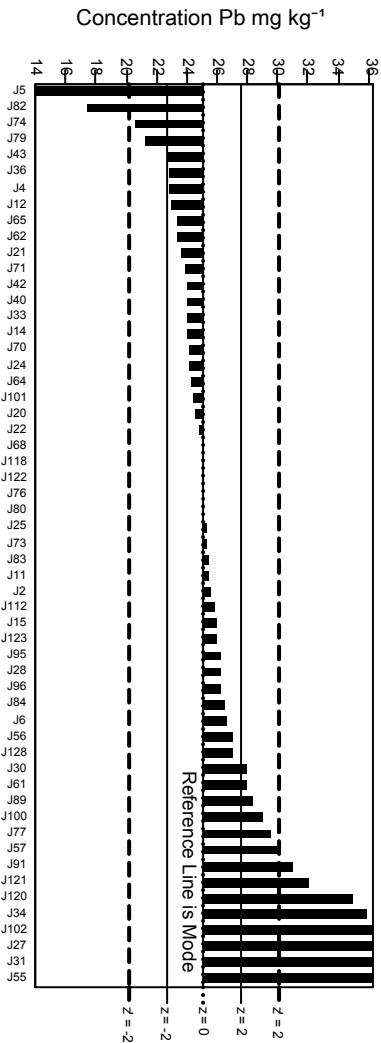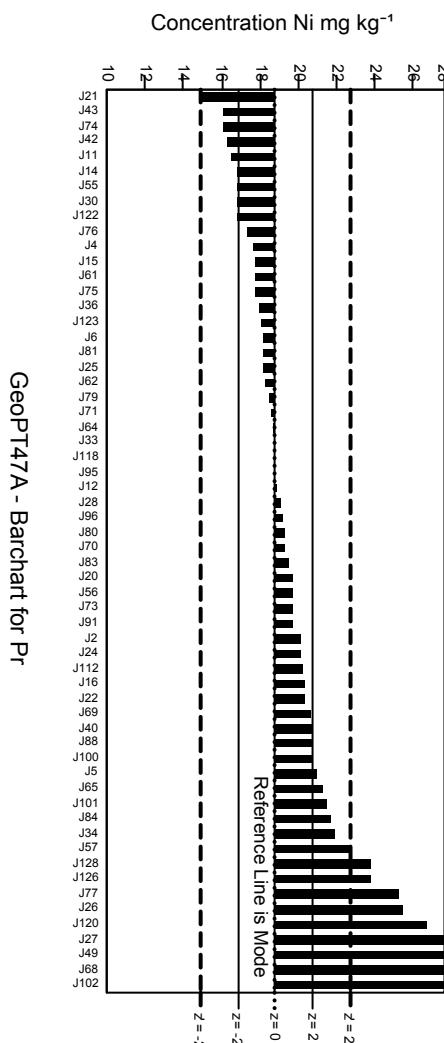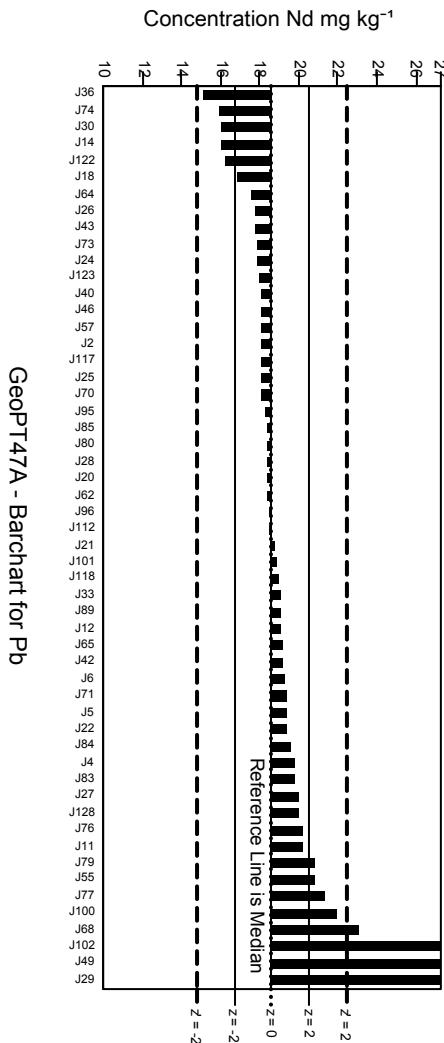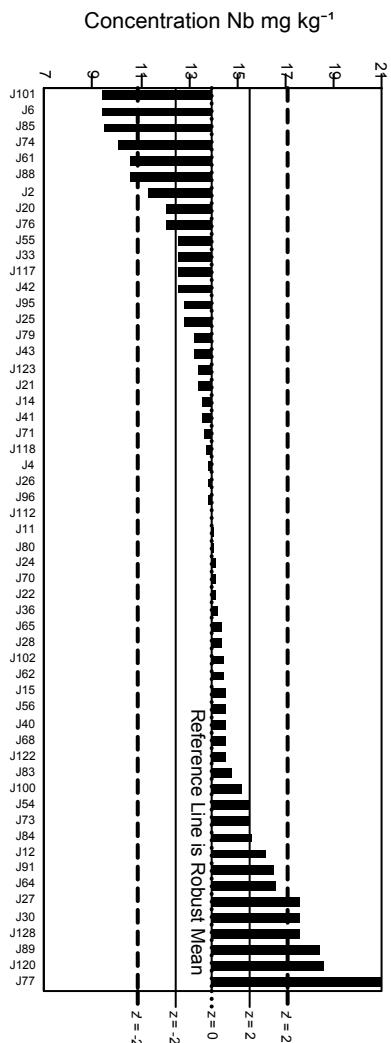


## GeoPT47A - Barchart for Rb

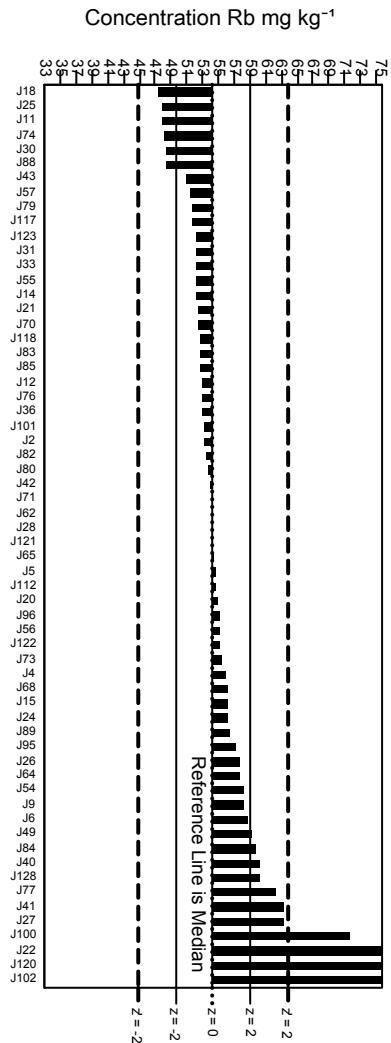


## GeoPT47A - Barchart for Sb

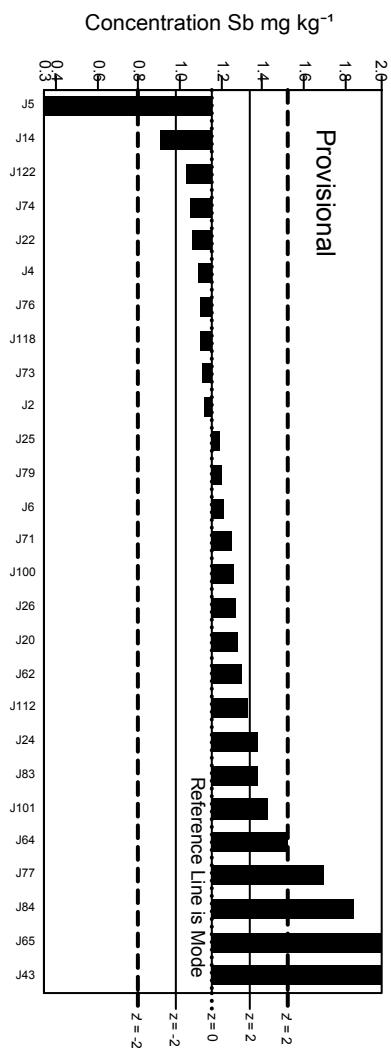


## Concentration Sc $\text{mg kg}^{-1}$

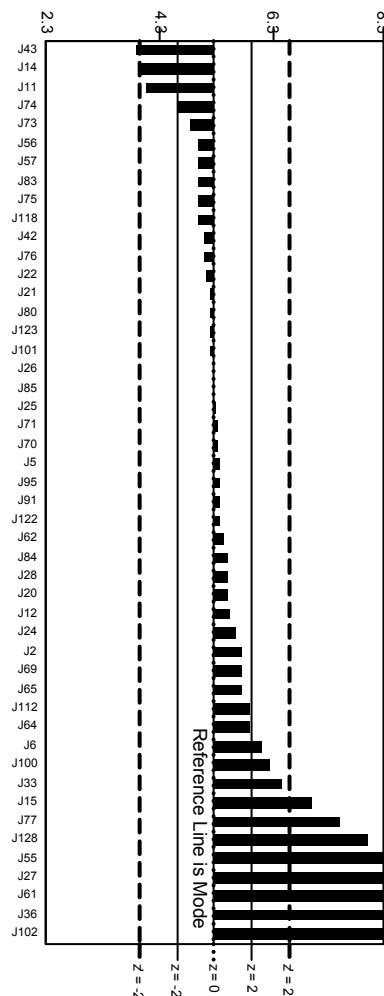


## GeoPT47A - Barchart for Sn

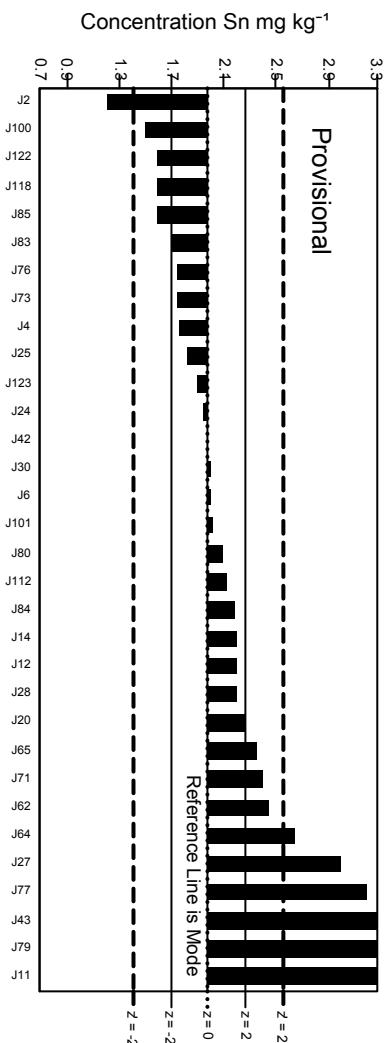


## GeoPT47A - Barchart for Sr

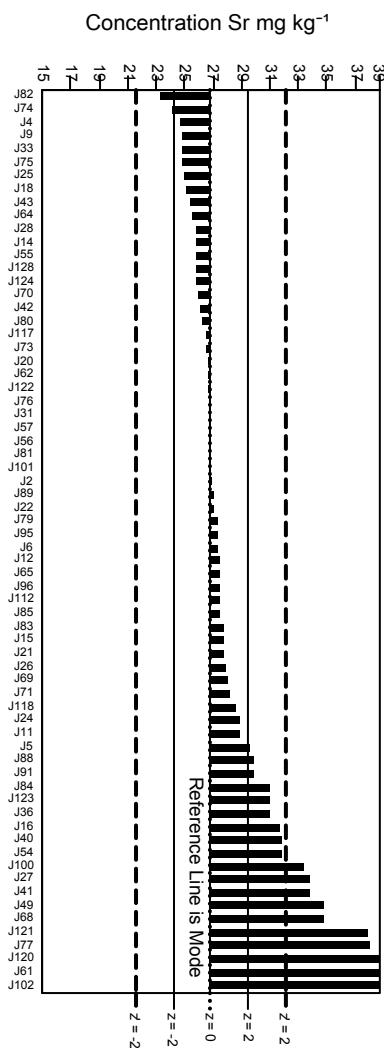


### GeoPT47A - Barchart for Ta

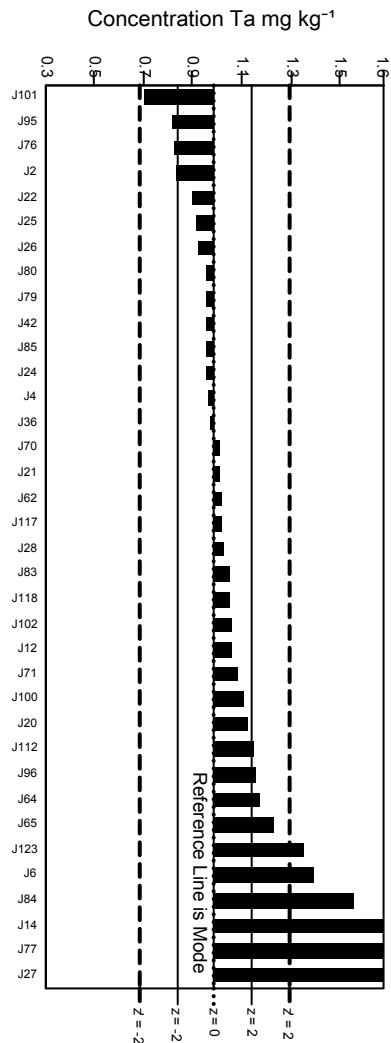


### GeoPT47A - Barchart for Th

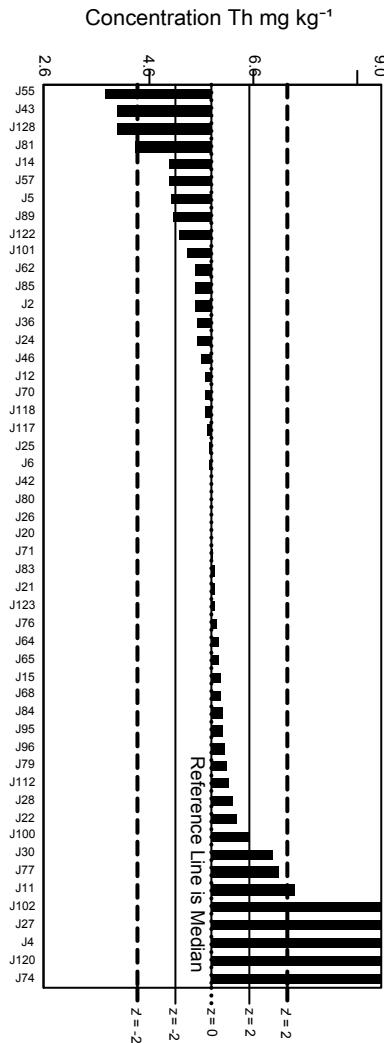


### GeoPT47A - Barchart for Tm

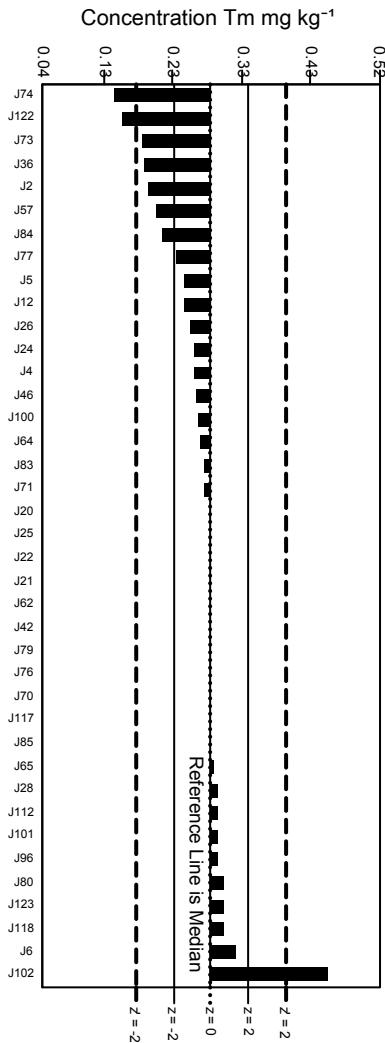

### GeoPT47A - Barchart for Tb

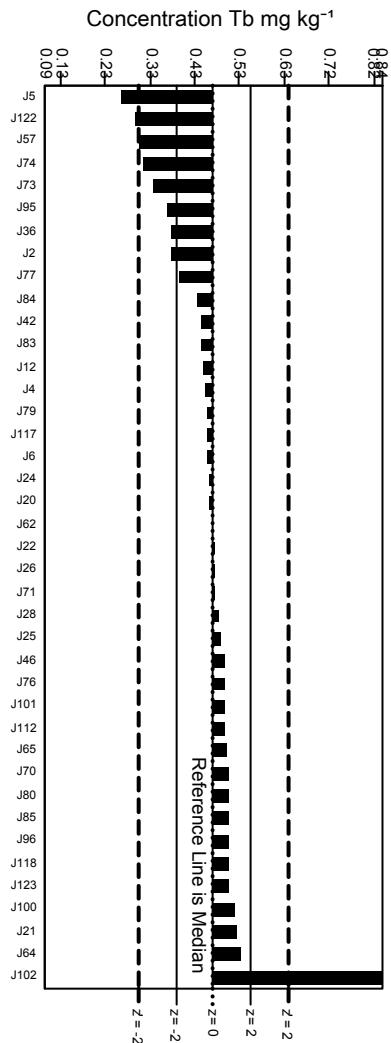

### GeoPT47A - Barchart for U

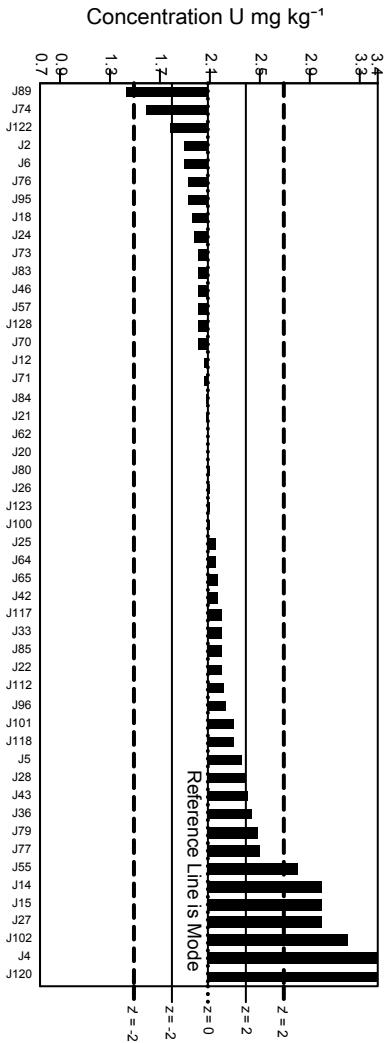



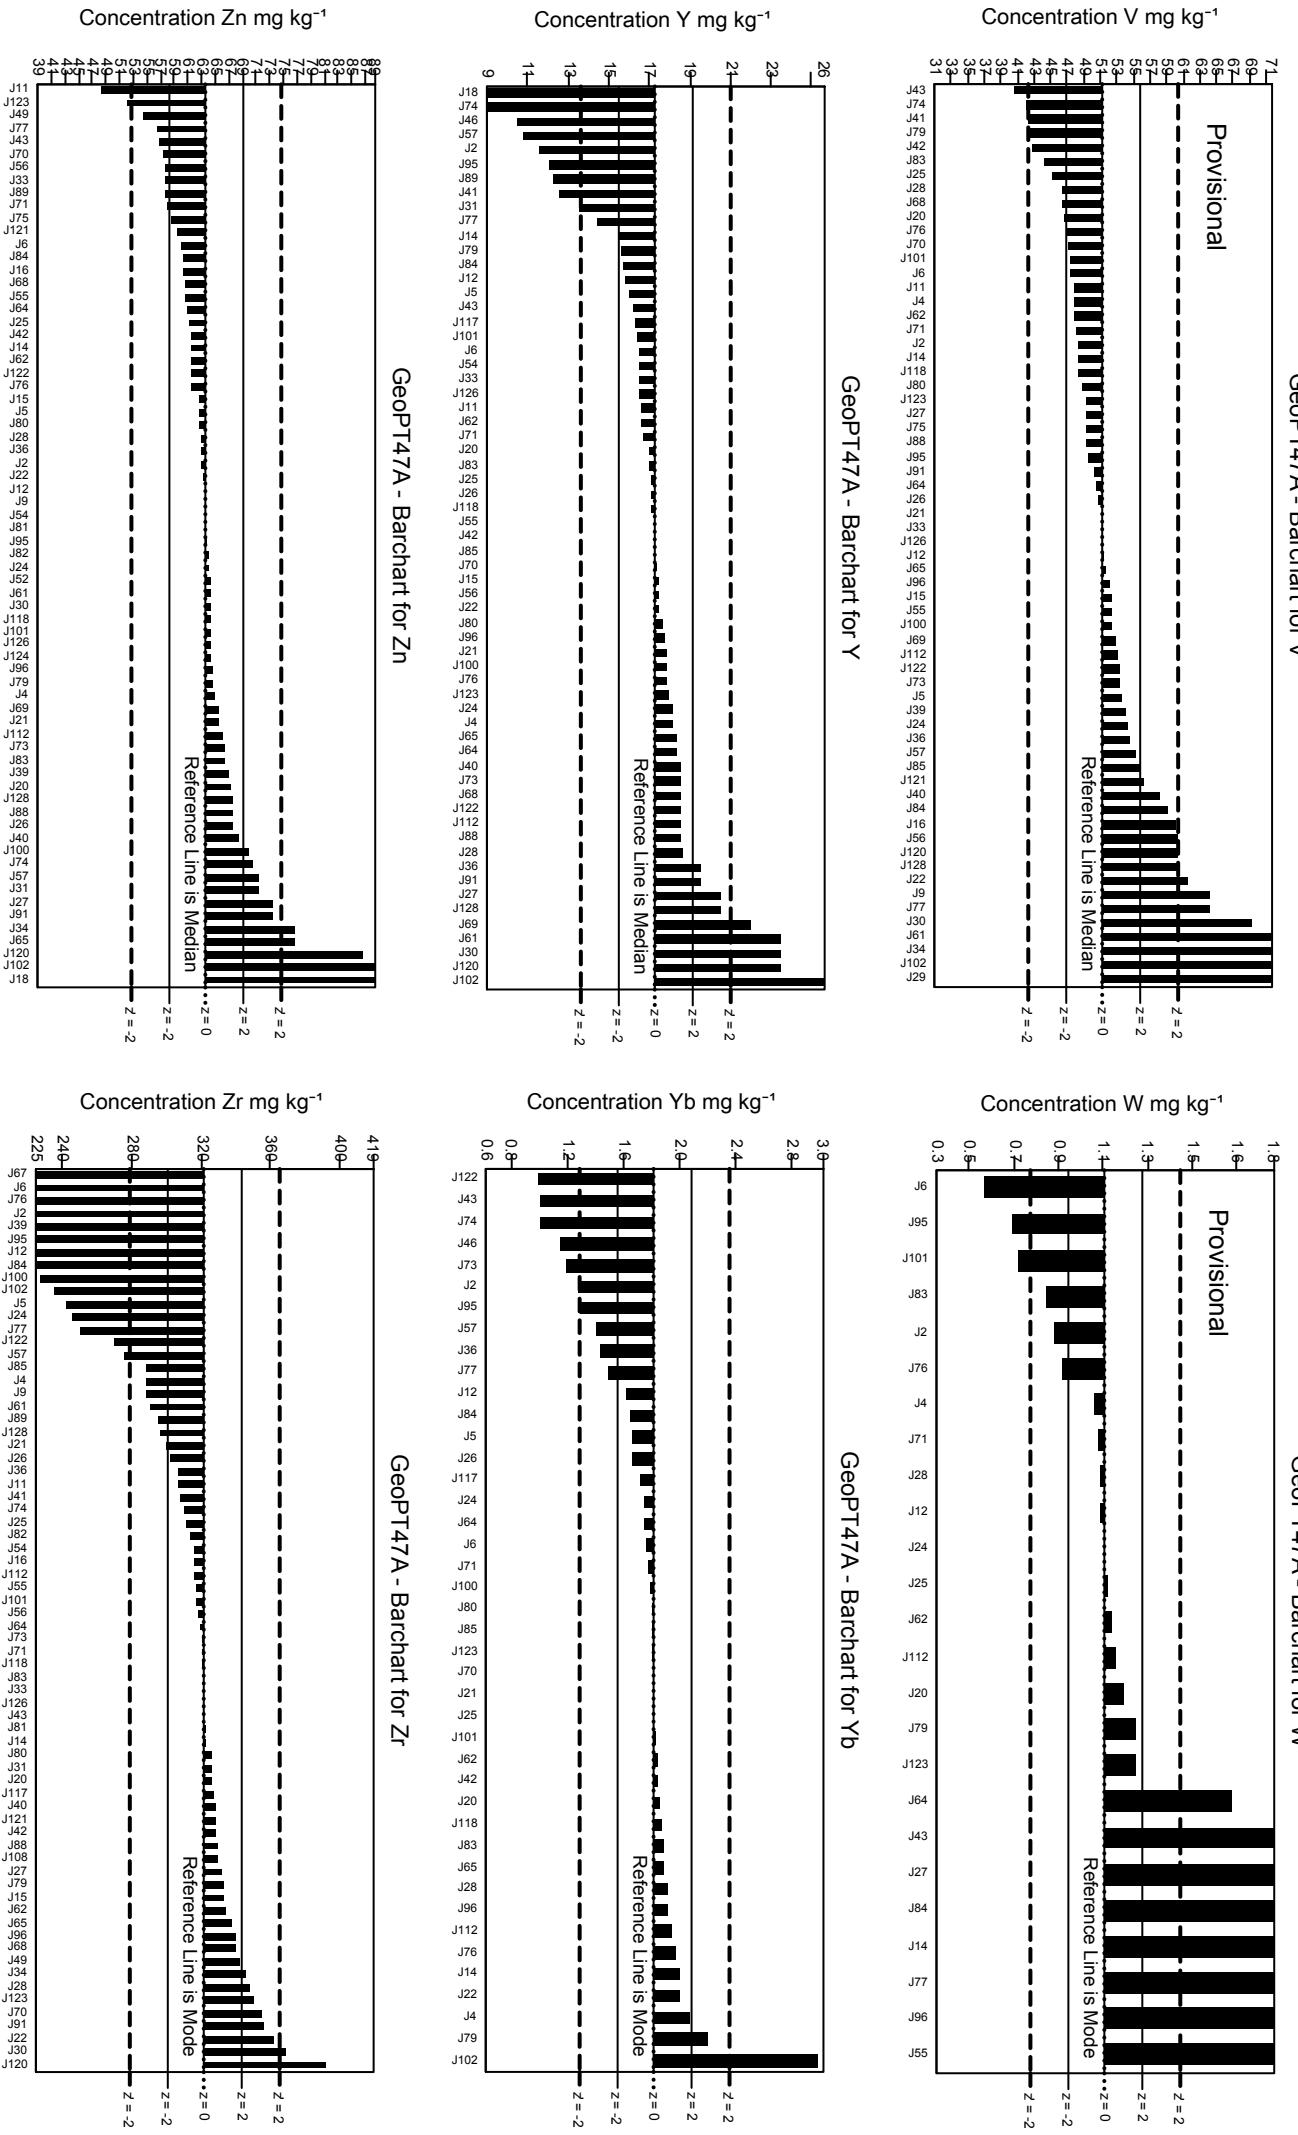


Figure 1: GeoPT47A - Silty soil, NES-1. Data distribution charts for elements for which values were assigned or provisional values given for guidance. Horizontal lines show the limits for -2<Z<2 for pure geochemistry labs (solid lines) and -2<Z<2 for applied geochemistry labs (pecked lines).


GeoPT47A - Barchart for Fe(II)O

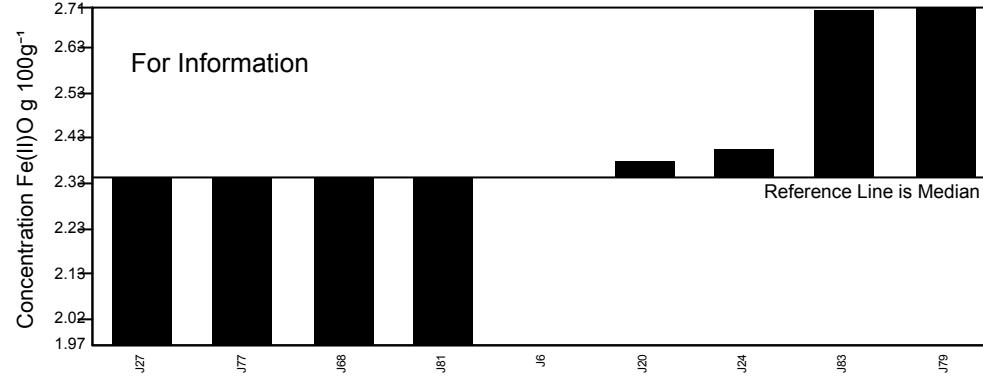


GeoPT47A - Barchart for Na2O

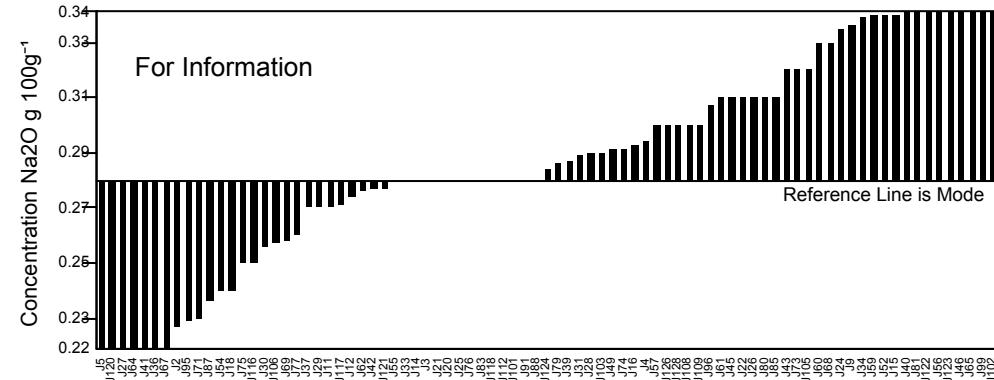


GeoPT47A - Barchart for C(tot)

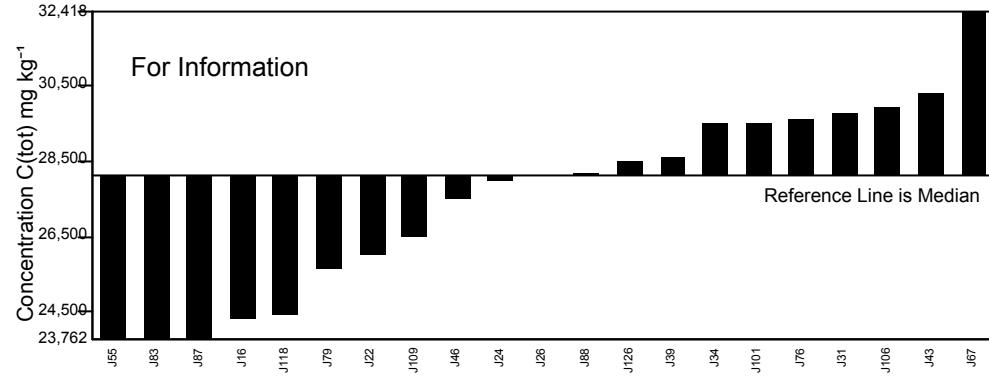


GeoPT47A - Barchart for Cl

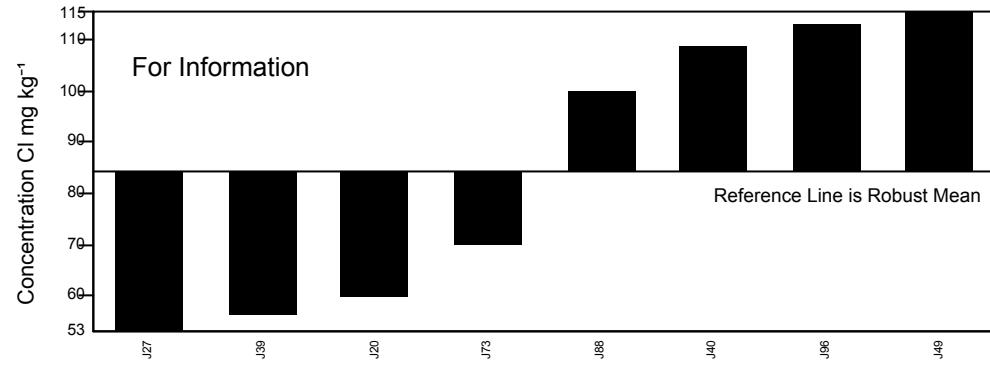


GeoPT47A - Barchart for F

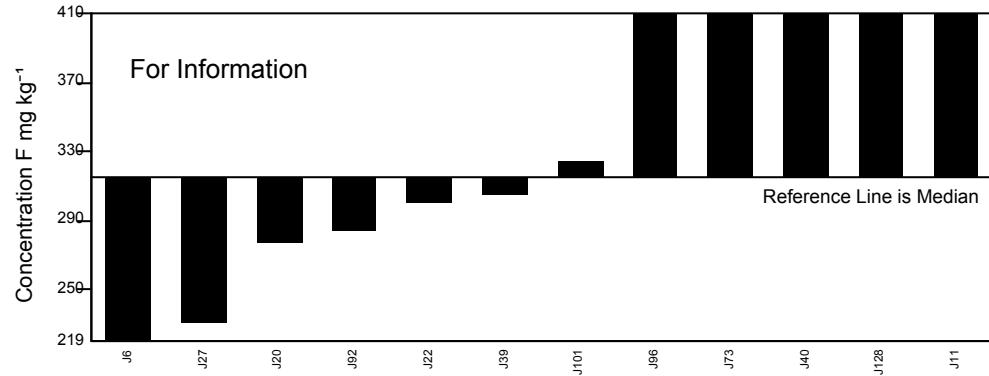


GeoPT47A - Barchart for Ge

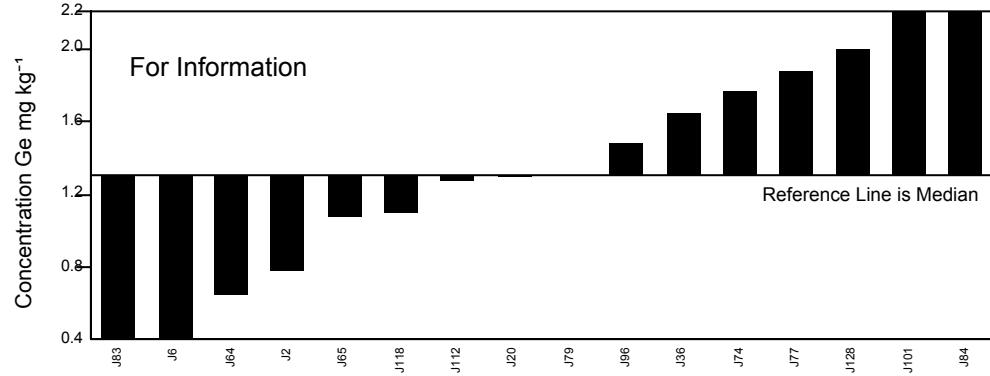


GeoPT47A - Barchart for Hg

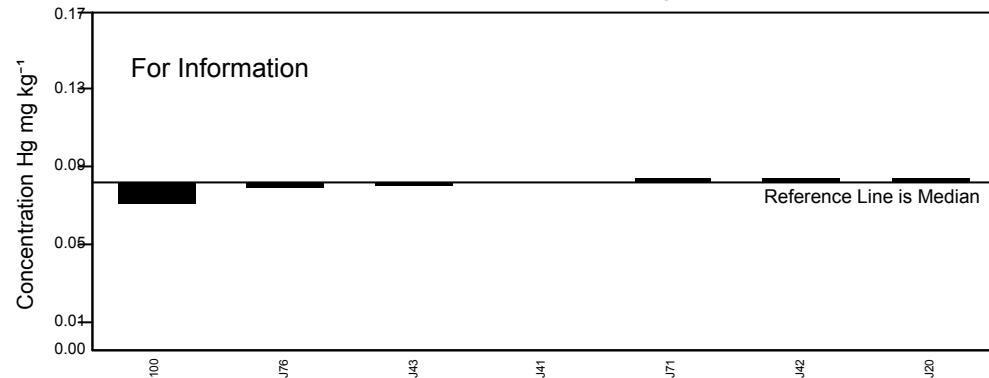


GeoPT47A - Barchart for In

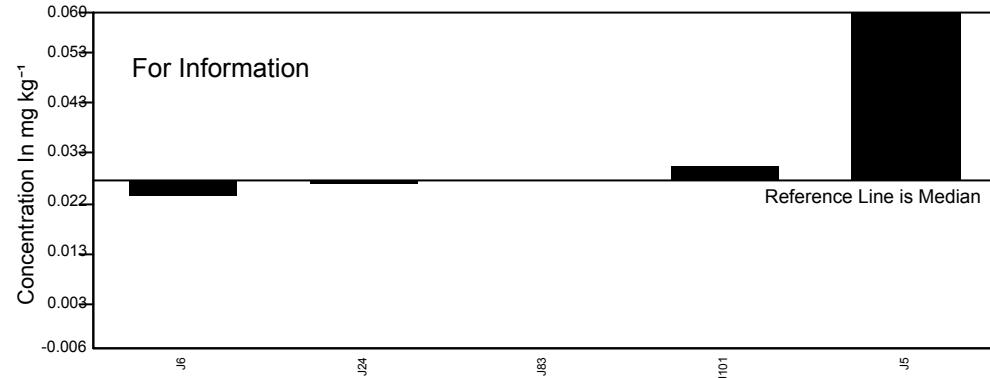

GeoPT47A - Barchart for S

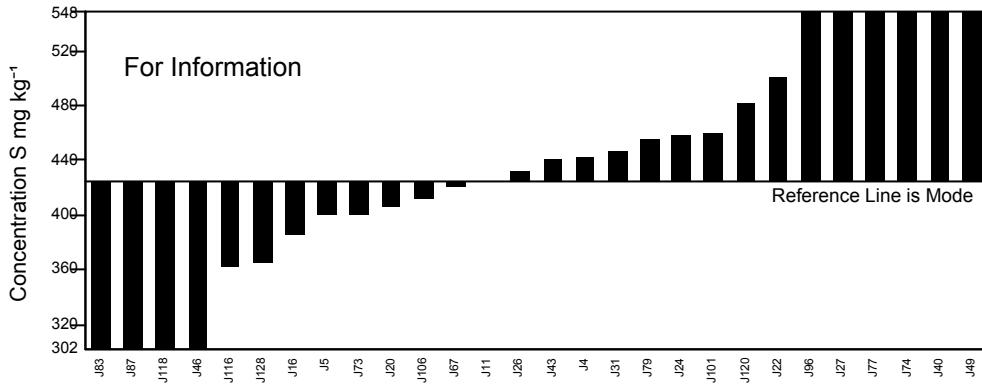

GeoPT47A - Barchart for Se

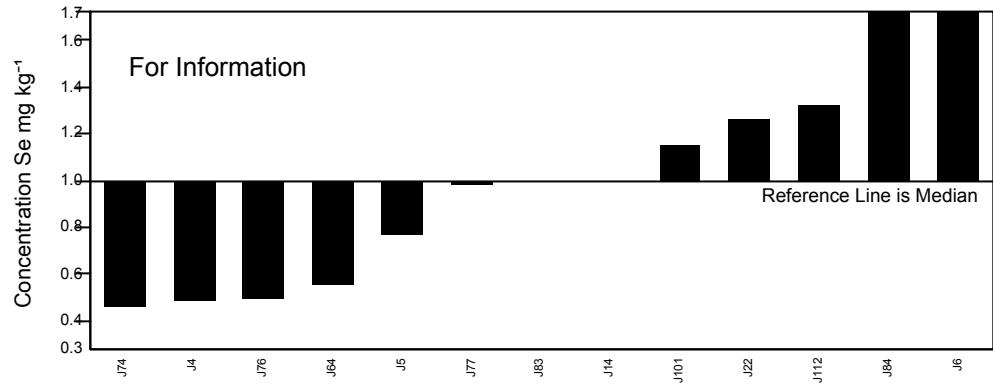

GeoPT47A - Barchart for Te

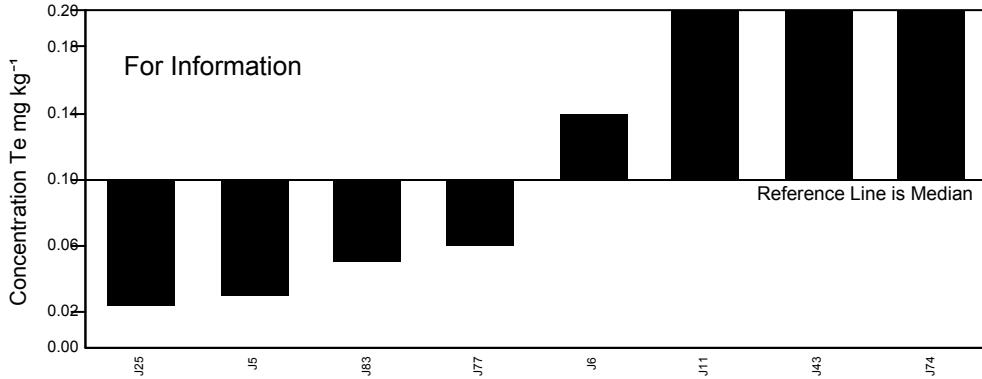
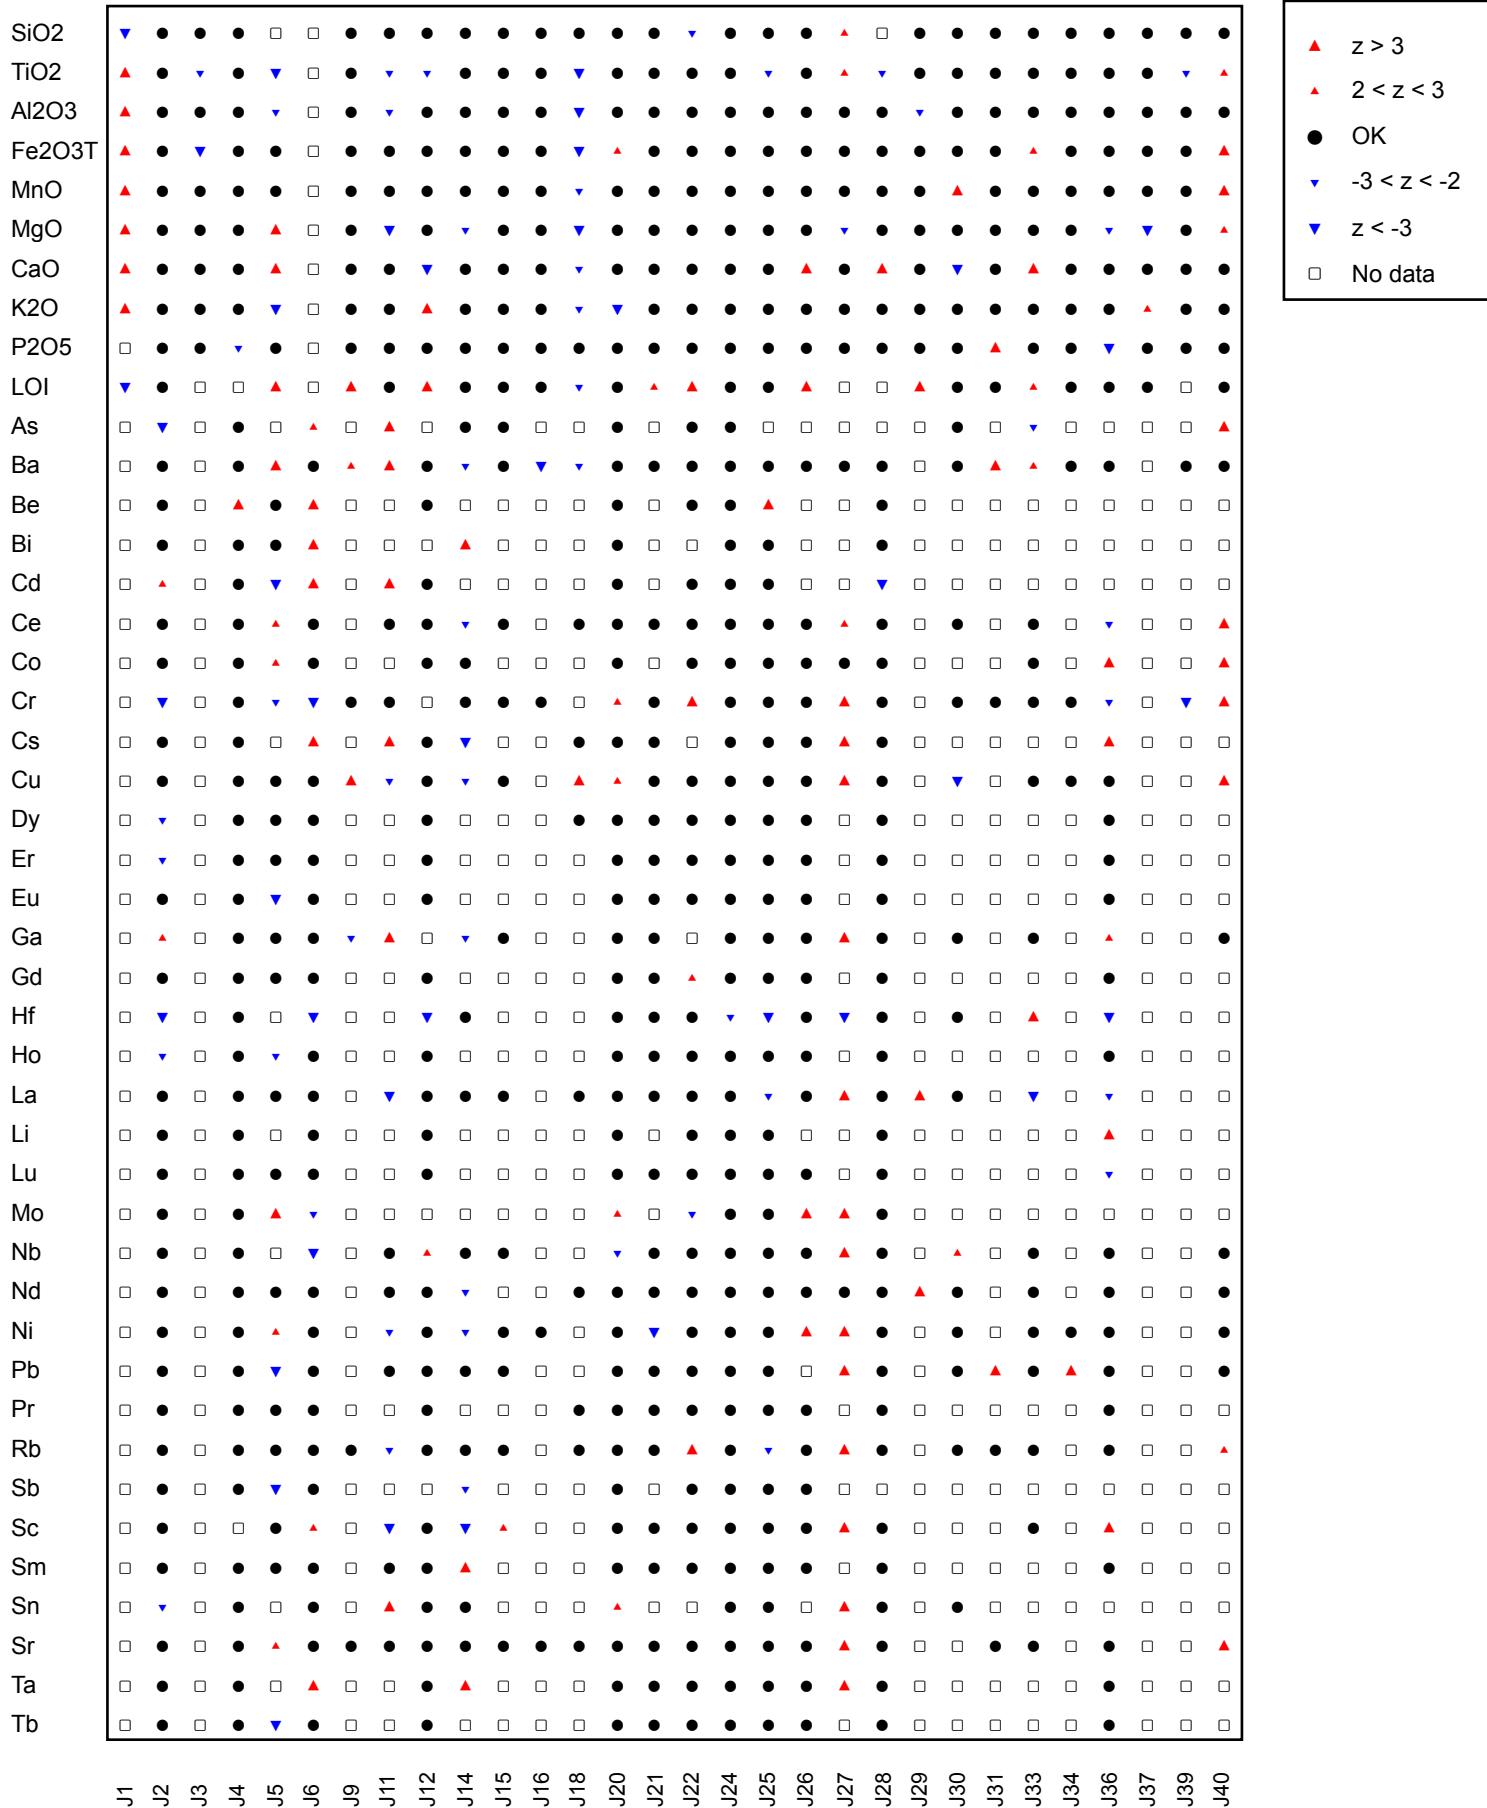


Figure 2: GeoPT47A - Silty soil, NES-1. Data distribution charts provided for information only for elements for which values could not be assigned.

### Multiple Z-Score Chart for GeoPT47A



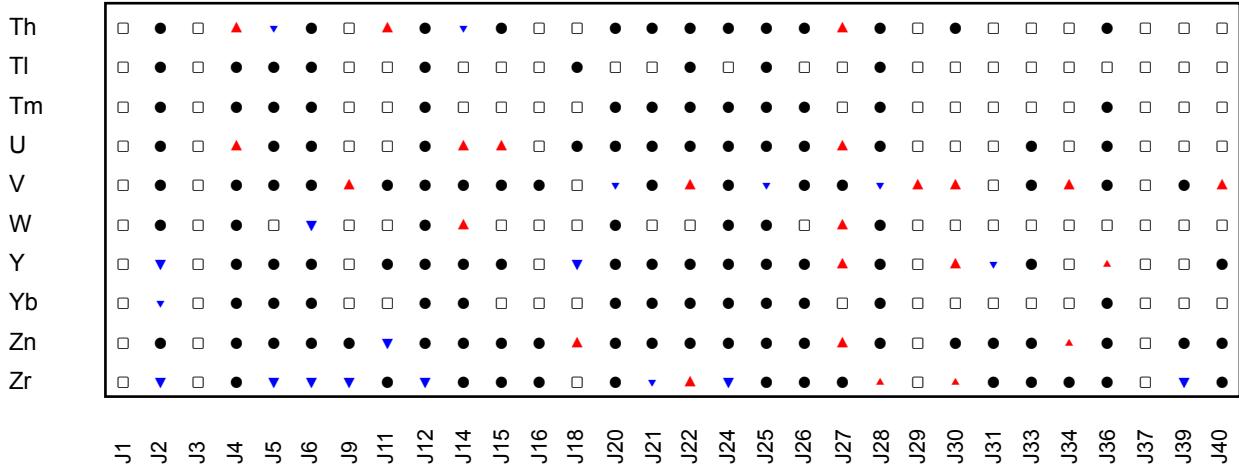
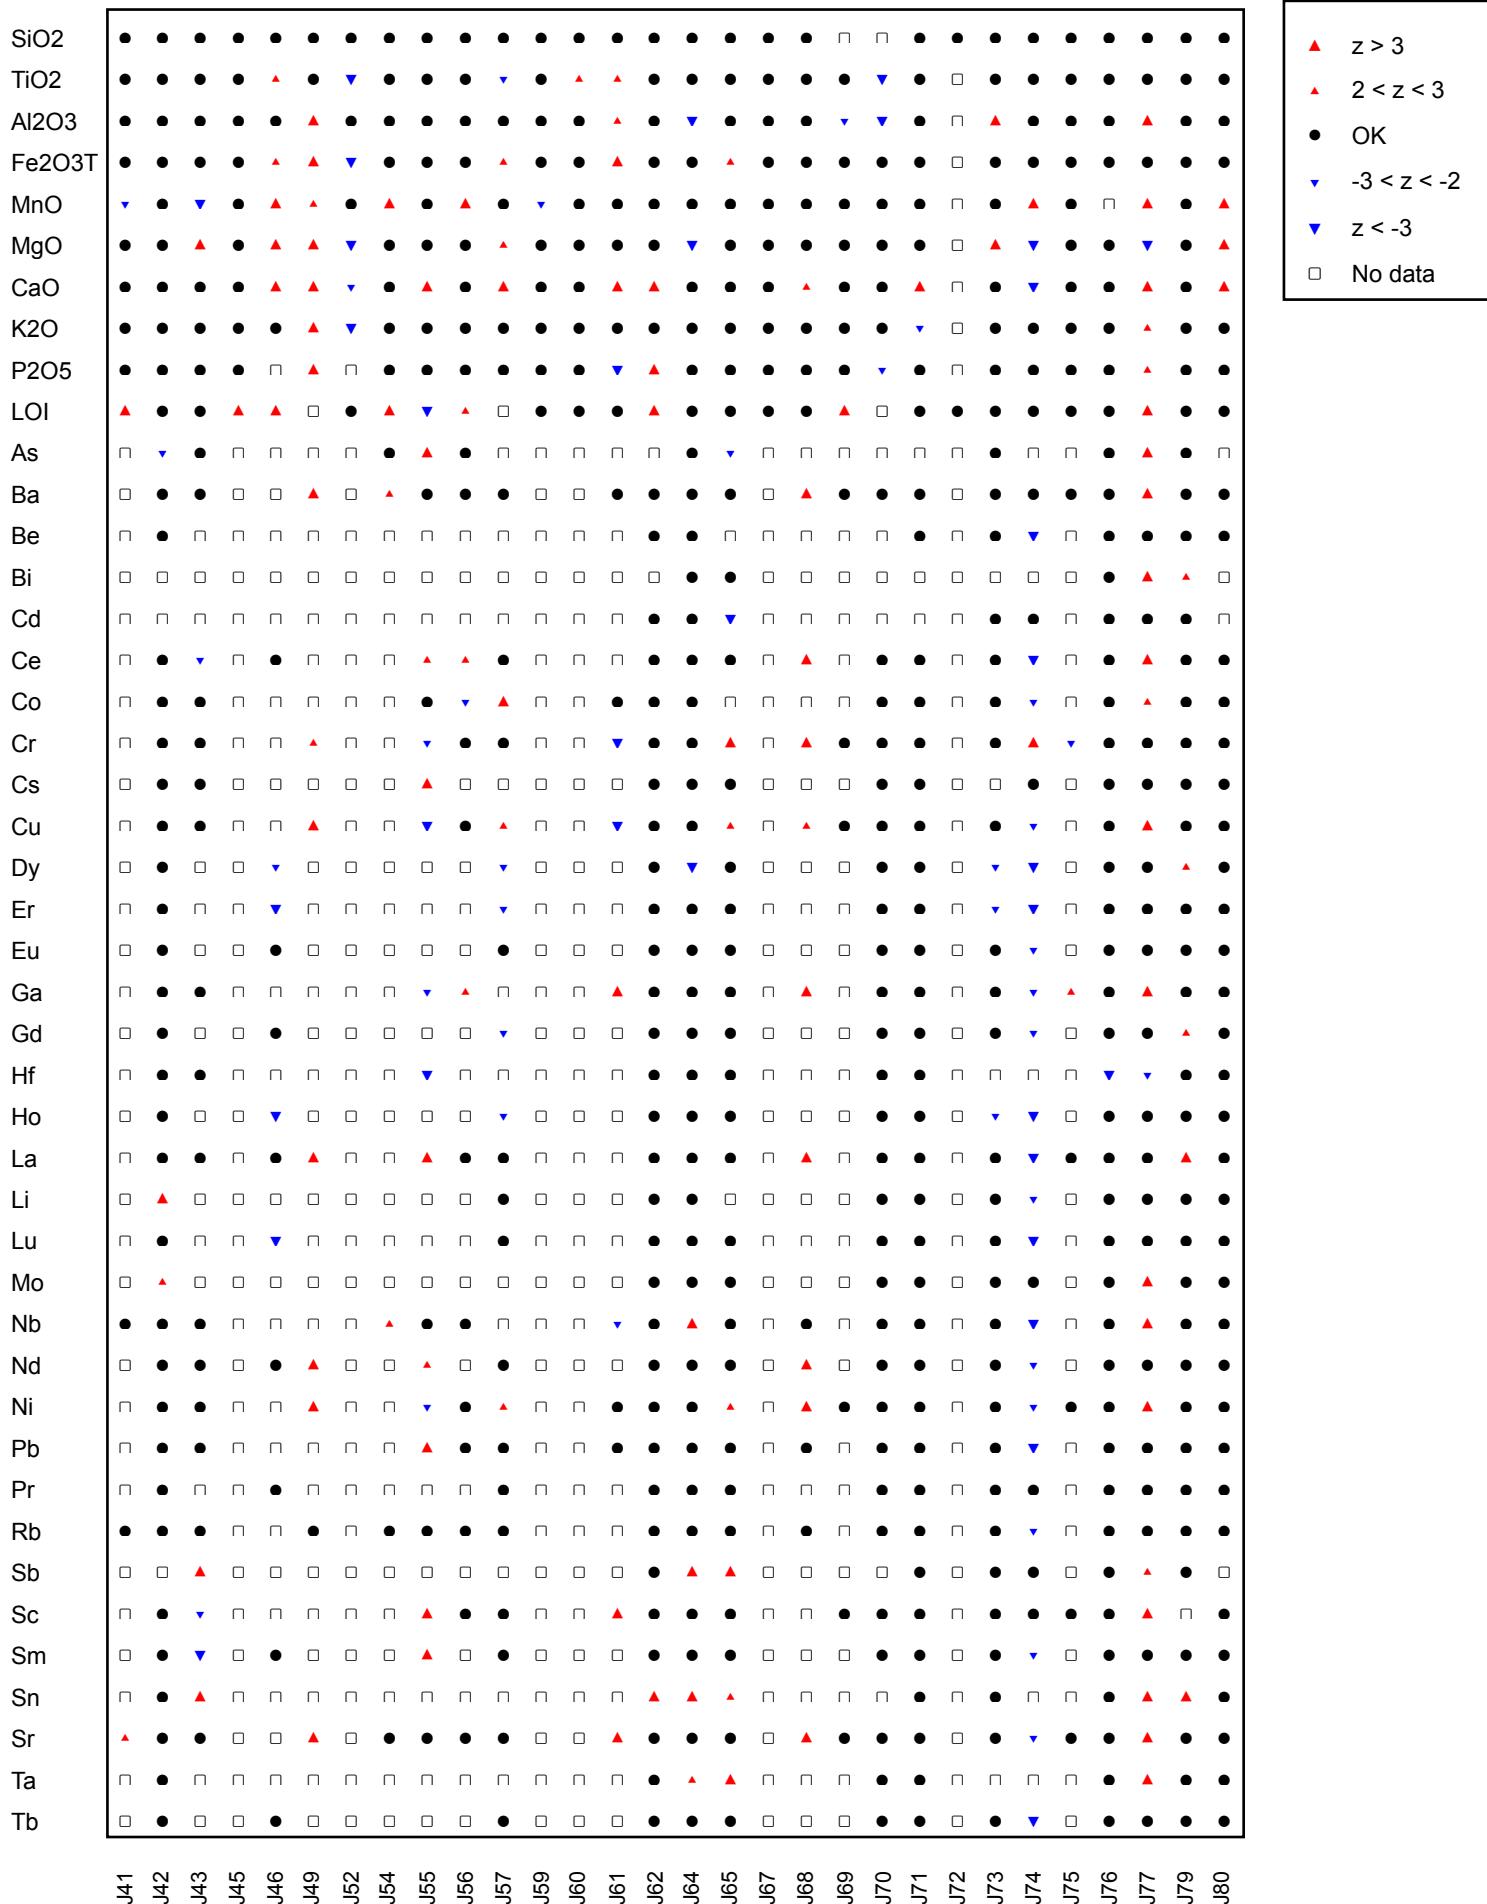


Figure 3: GeoPT47A - Silty soil, NES-1. Multiple z-score charts for laboratories participating in the GeoPT47 A round. Symbols indicate whether or not an elemental result complies with the  $-2 < z < +2$  criteria (see key).

### Multiple Z-Score Chart for GeoPT47A



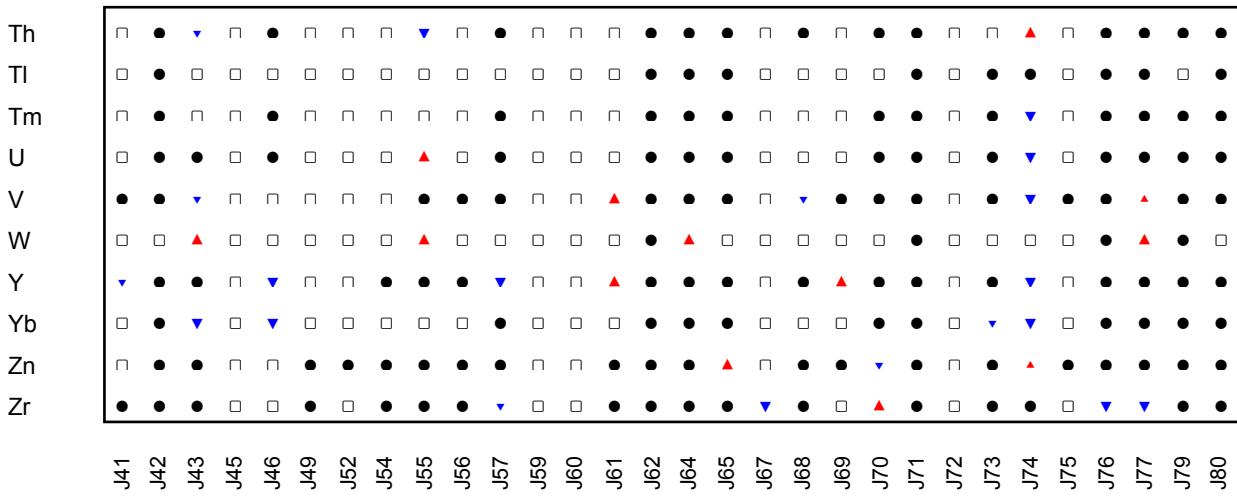
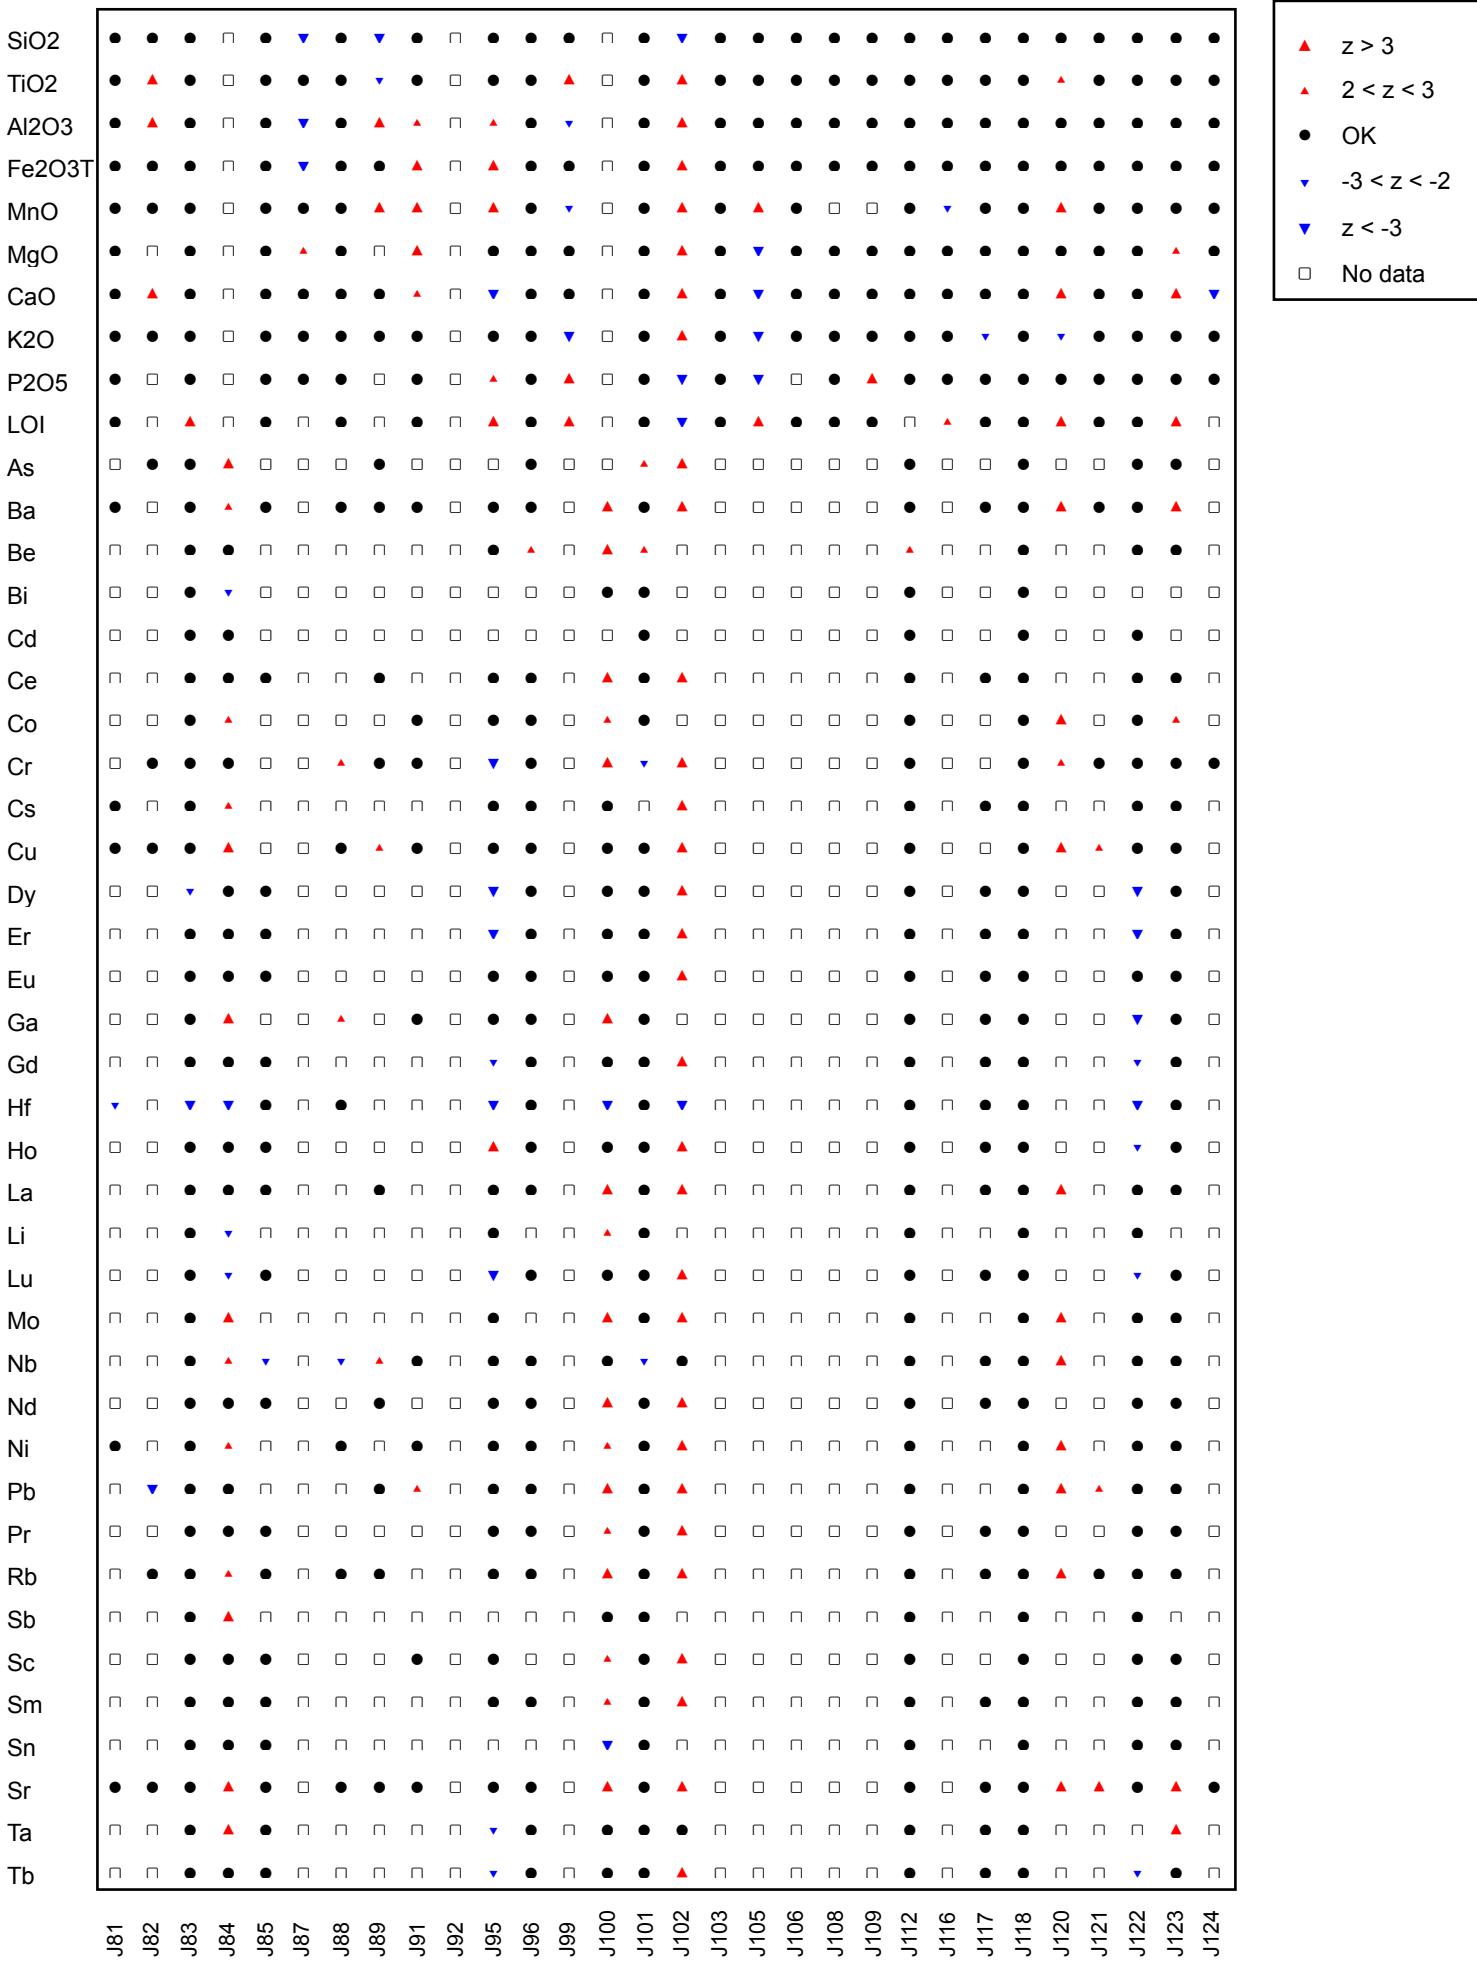


Figure 3: GeoPT47A - Silty soil, NES-1. Multiple z-score charts for laboratories participating in the GeoPT47 A round. Symbols indicate whether or not an elemental result complies with the  $-2 < z < +2$  criteria (see key).

### Multiple Z-Score Chart for GeoPT47A




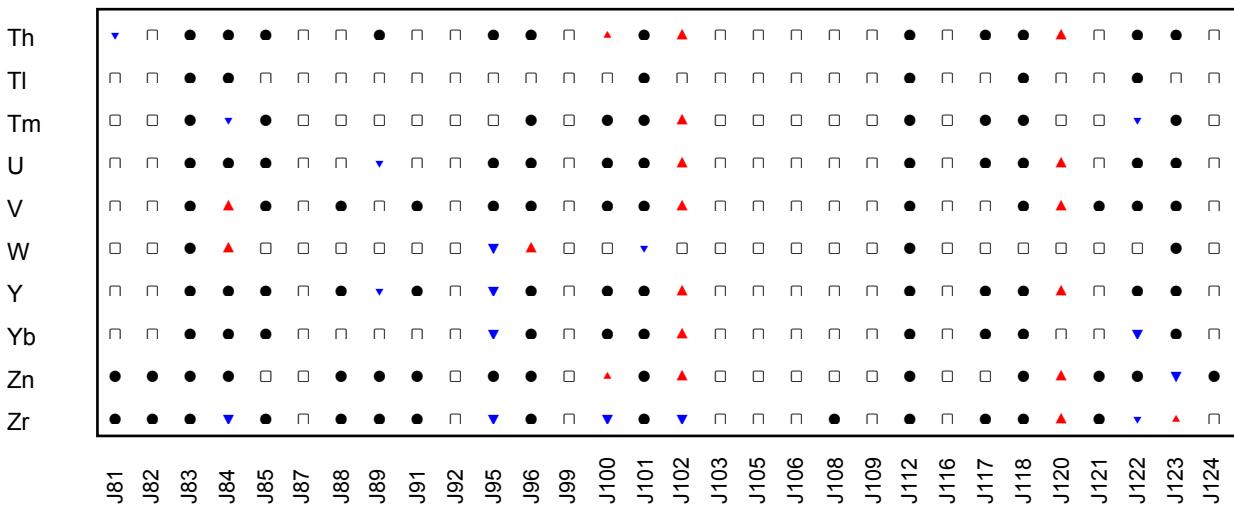


Figure 3: GeoPT47A - Silty soil, NES-1. Multiple z-score charts for laboratories participating in the GeoPT47 A round. Symbols indicate whether or not an elemental result complies with the  $-2 < z < +2$  criteria (see key).

### Multiple Z-Score Chart for GeoPT47A



J126 J128

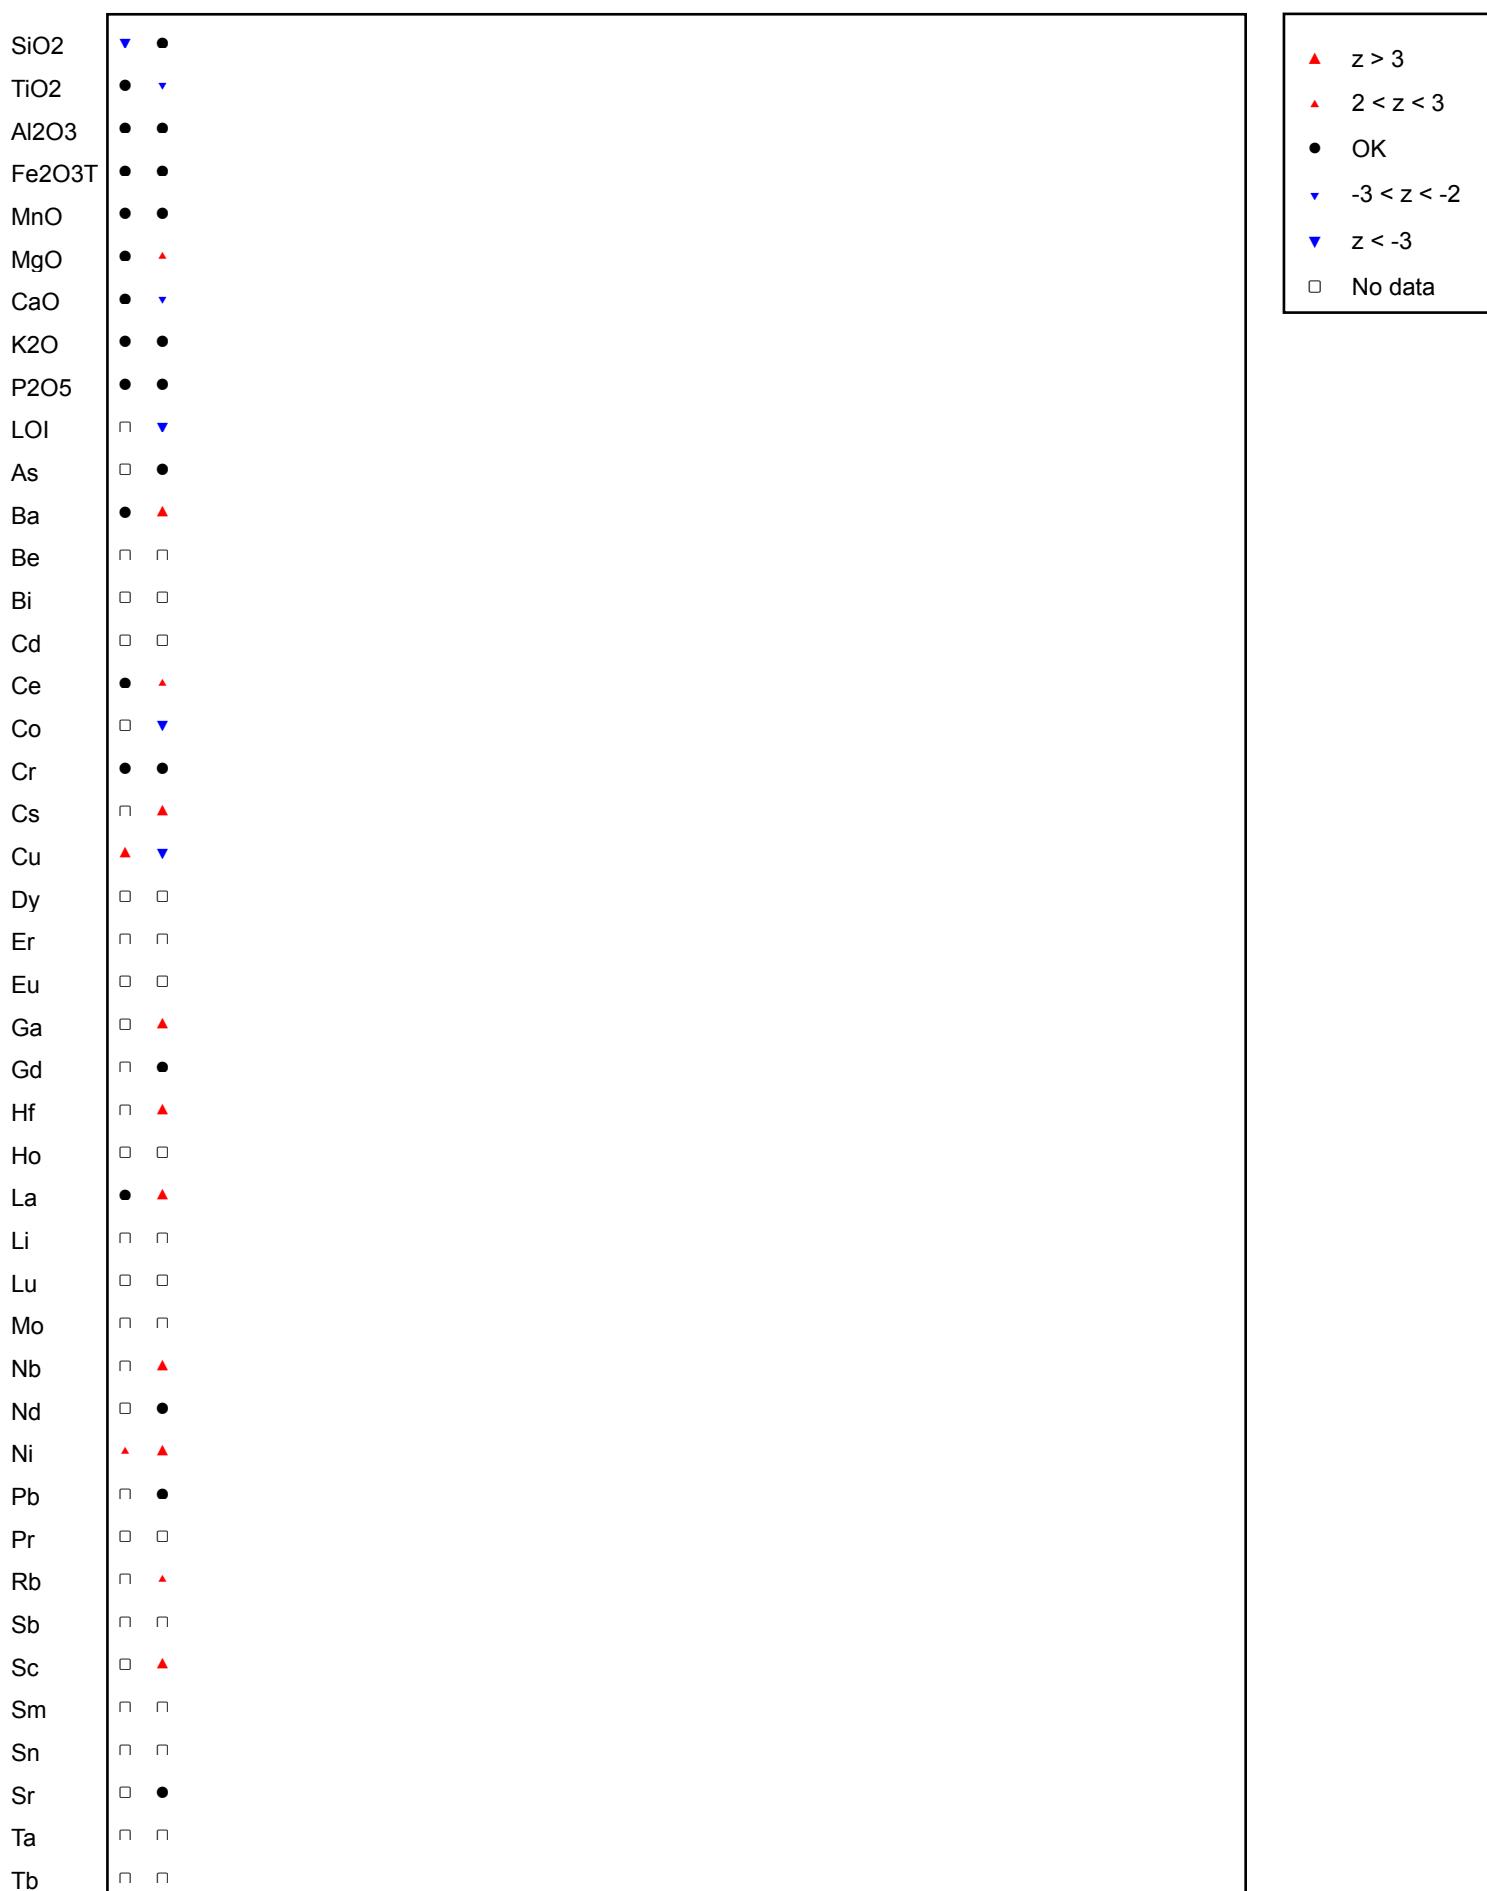

J126  
J128

Figure 3: GeoPT47A - Silty soil, NES-1. Multiple z-score charts for laboratories participating in the GeoPT47 A round. Symbols indicate whether or not an elemental result complies with the  $-2 < z < +2$  criteria (see key).